

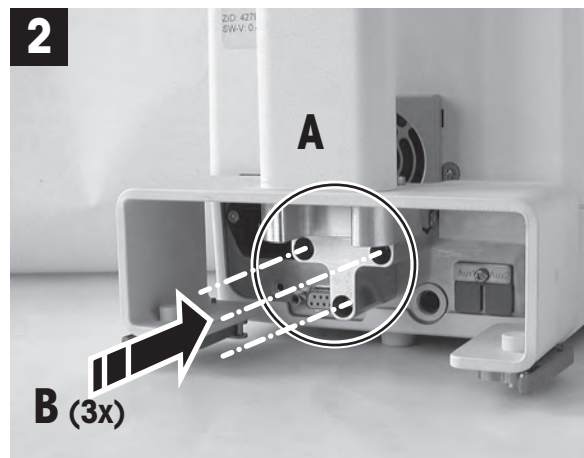
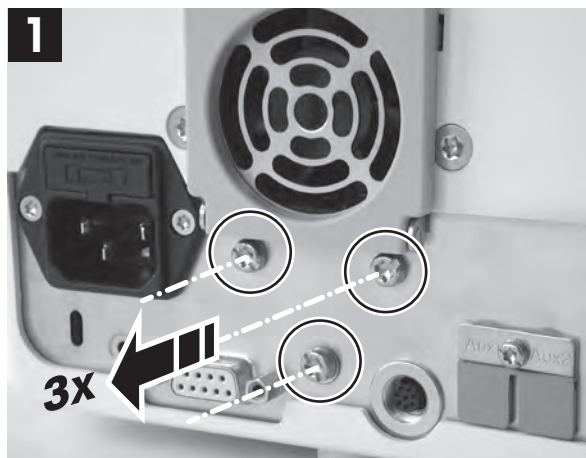
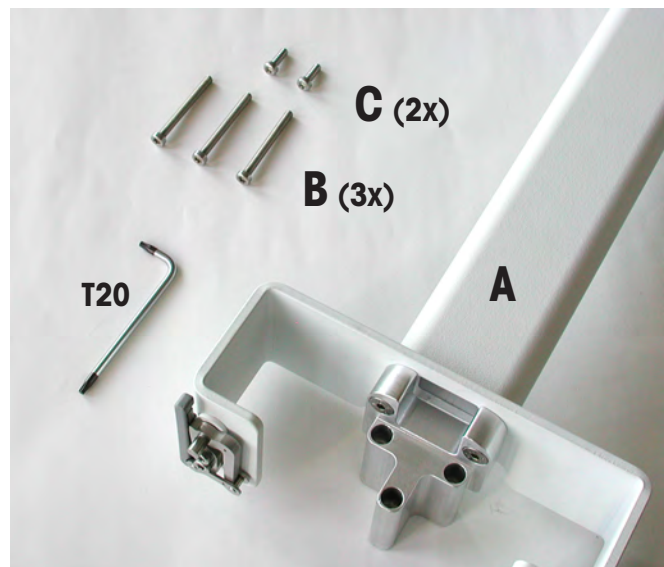
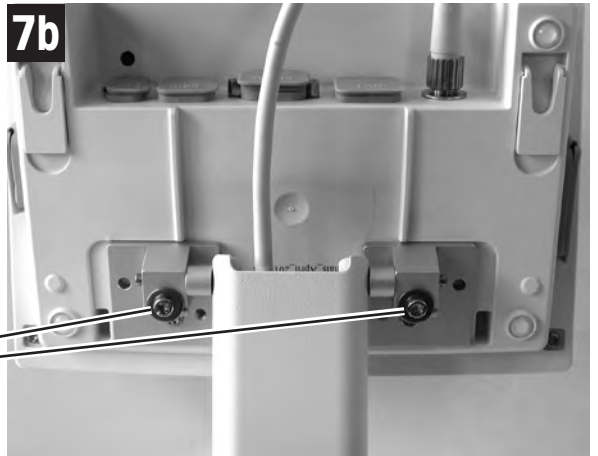
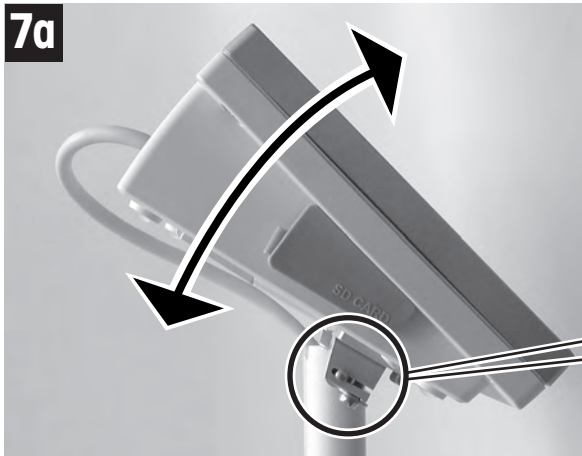
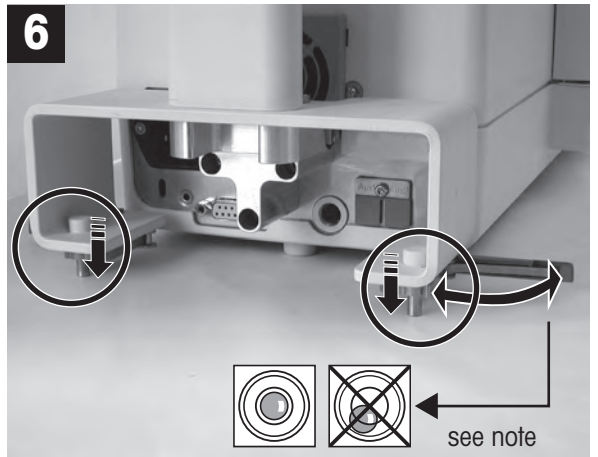
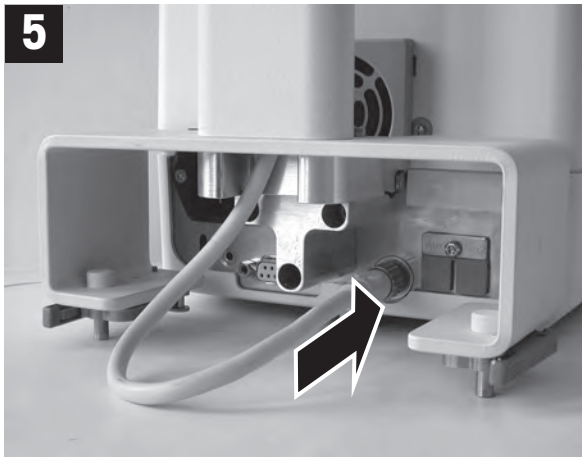


Stand for Terminal HX/HS Moisture Analyzer

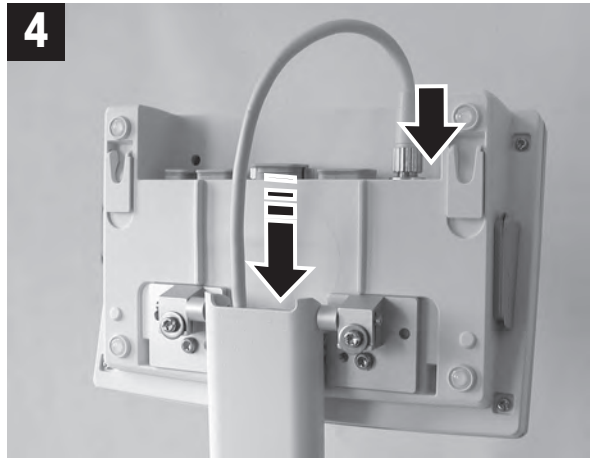

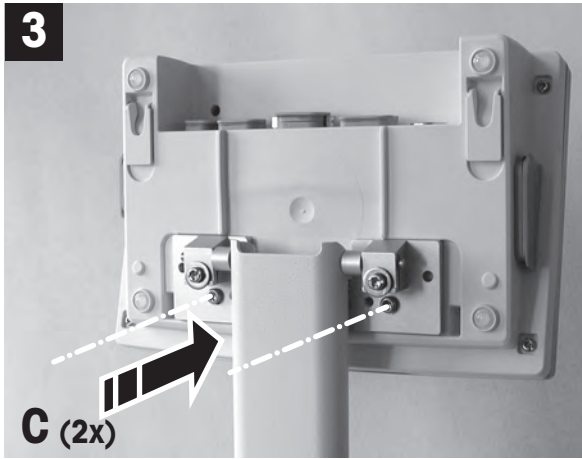

Note: For leveling the drying unit see Reference Manual

www.mt.com/HX204-RM

www.mt.com/HS153-RM

www.mt.com/moisture

For more information

Mettler-Toledo GmbH
 Im Langacher
 8606 Greifensee, Switzerland
www.mt.com/contact

Subject to technical changes
 © Mettler-Toledo GmbH 07/2021
 30024233A en

