

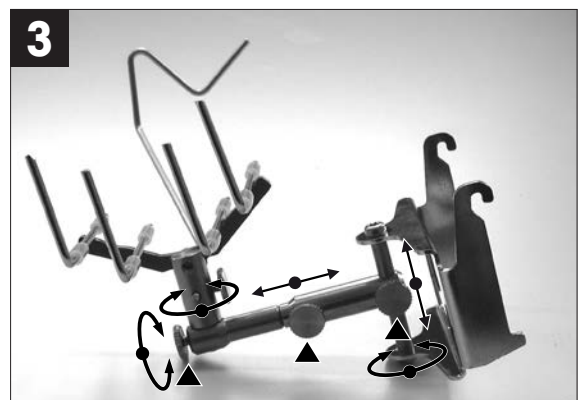
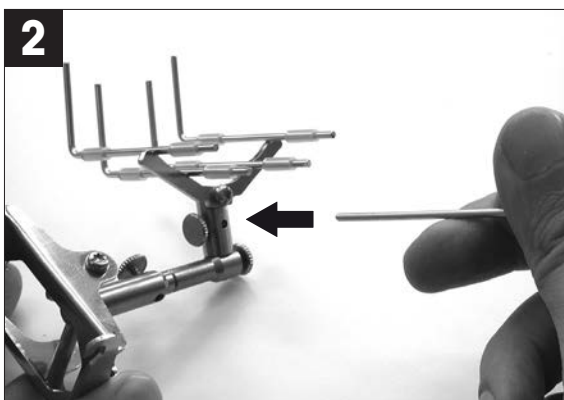
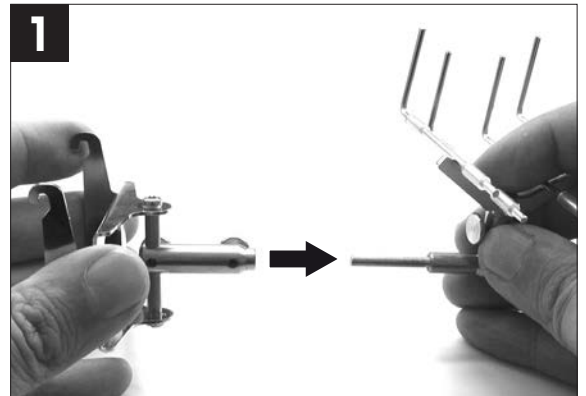


# ErgoClip Flask



for Analytical Balances XP, XS, XA, XPE, XSE

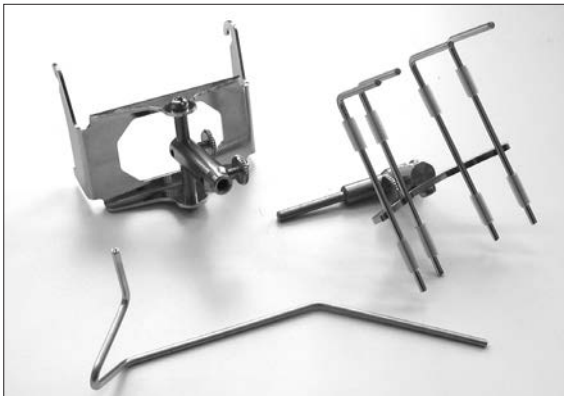

**4**

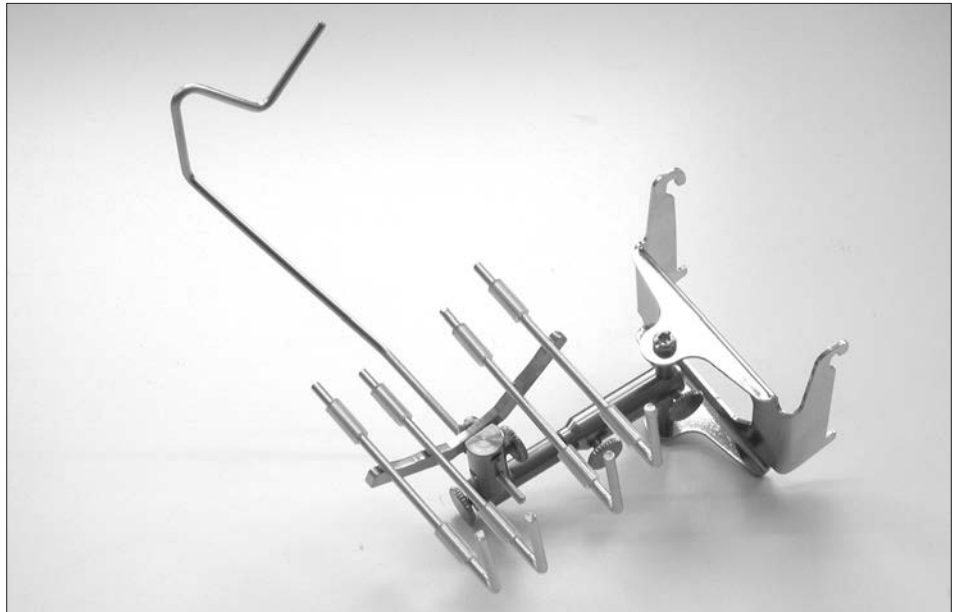


**OFF**

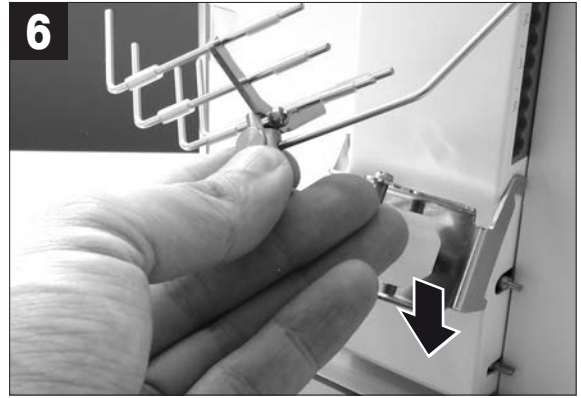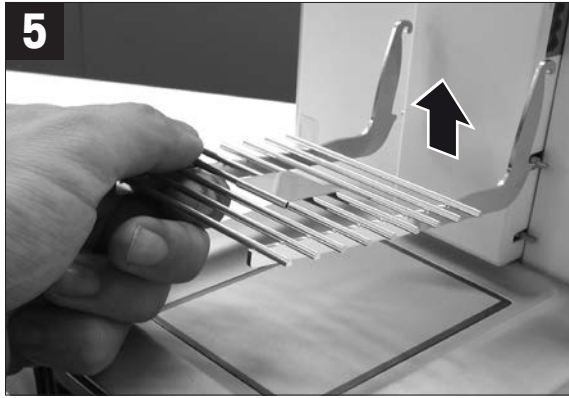

**8**




**ON**

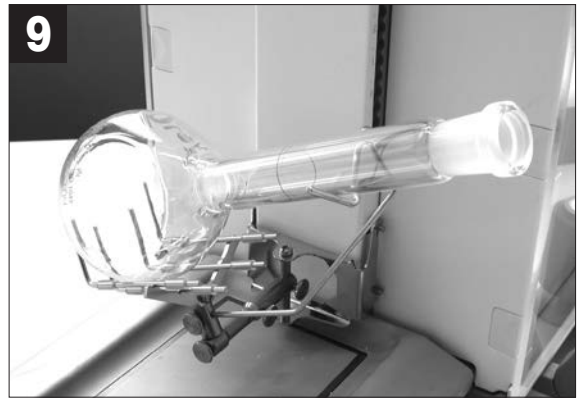

**10**

**→T←**

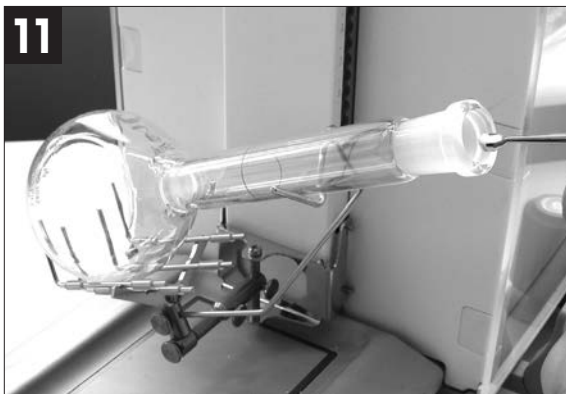

[www.mt.com/lab-accessories](http://www.mt.com/lab-accessories)

For more information

**Mettler-Toledo AG, Laboratory Weighing**  
CH-8606 Greifensee, Switzerland  
Phone +41 44 944 22 11  
Fax +41 44 944 30 60  
Internet: [www.mt.com](http://www.mt.com)

Subject to technical changes  
© Mettler-Toledo AG 07/2014  
11780812A ml

