

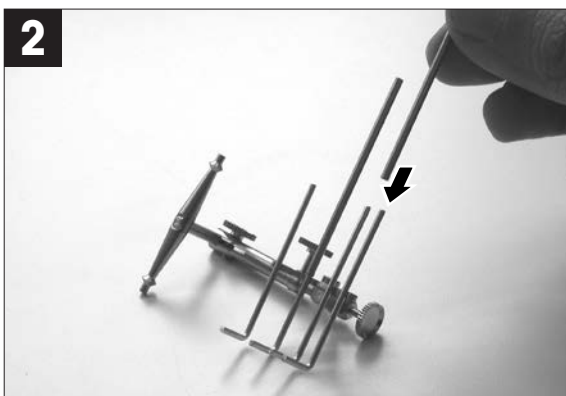
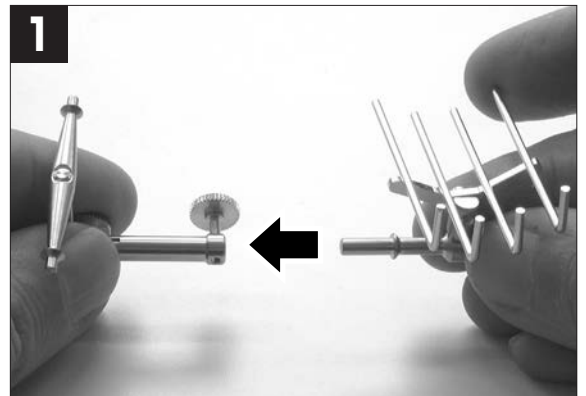
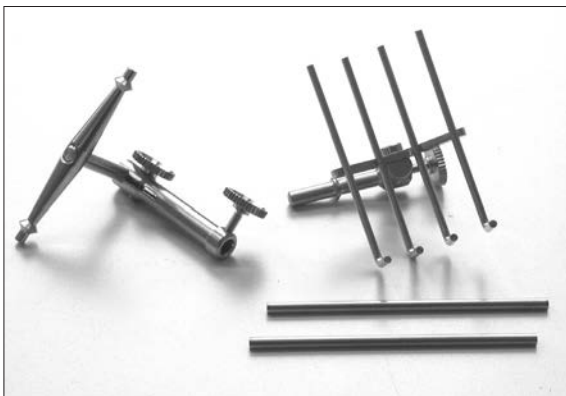
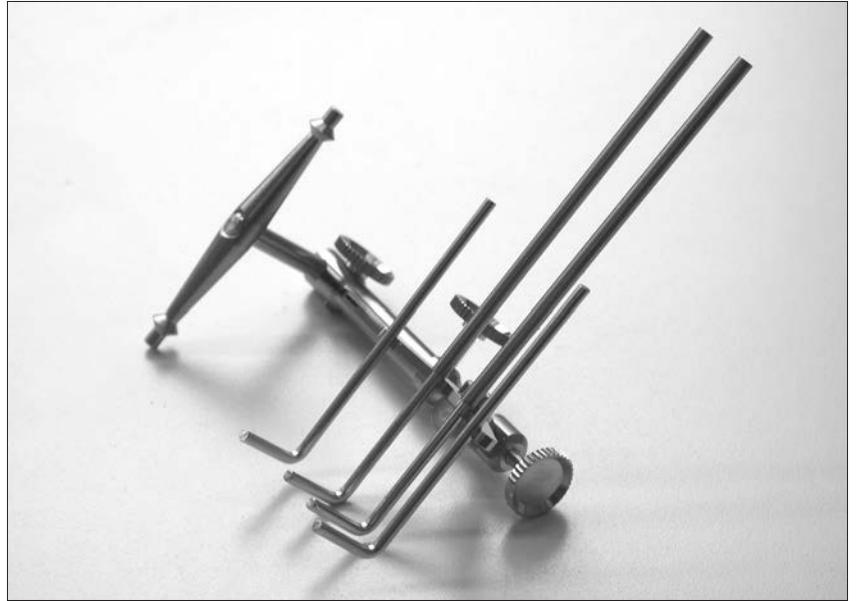
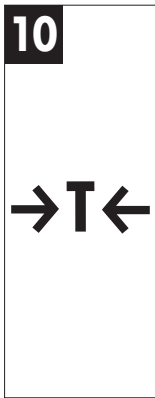
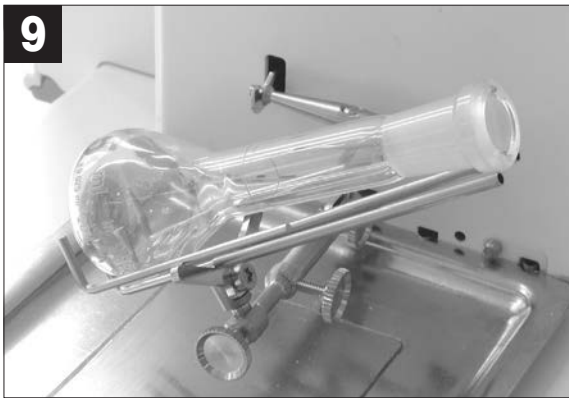
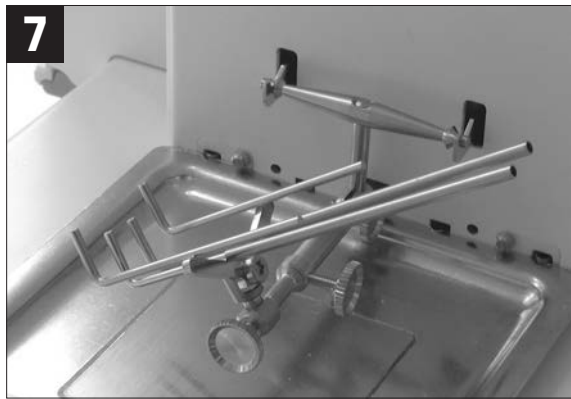
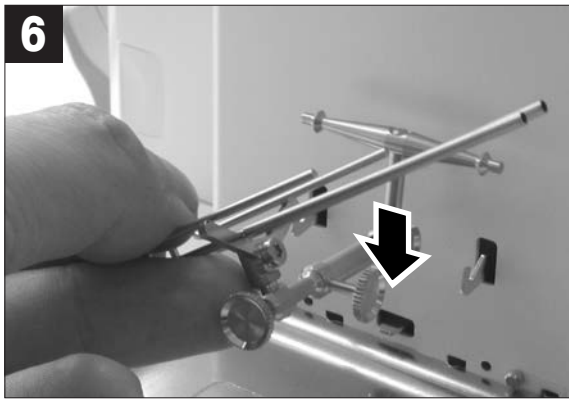


ErgoClip Flask Micro

for Micro Balances XP26/XP56, XPE26/XPE56

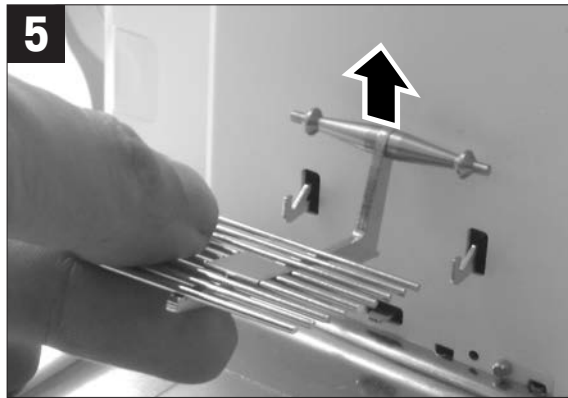

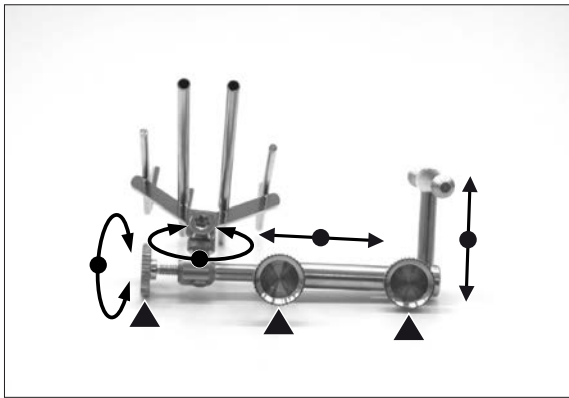

www.mt.com/lab-accessories

For more information

Mettler-Toledo AG, Laboratory Weighing
 CH-8606 Greifensee, Switzerland
 Phone +41 44 944 22 11
 Fax +41 44 944 30 60
 Internet: www.mt.com

Subject to technical changes
 © Mettler-Toledo AG 07/2014
 11780839A ml

