

Multi-Parameter Transmitter



METTLER TOLEDO

© It is forbidden to reprint this instruction manual in whole or part.

No part of this manual may be reproduced in any form, or modified, copied or distributed using electronic systems, in particular in the form of photocopies, photographs, magnetic or other recordings, without written consent of Mettler-Toledo GmbH, Process Analytics, CH-8902 Urdorf, Switzerland.

All rights reserved, in particular reproduction, translation and patenting/registration.

ISM is a trademark of the METTLER TOLEDO Group.

Operation Manual Multi-Parameter Transmitter M400 PA

Content

1	Introduction	9
1.1	Intended Use	9
2	Safety Instructions	10
2.1	Definition of Equipment and Documentation Symbols and Designations	10
2.2	Environmental protection	11
2.3	Ex Instructions for M400 Series Multi-parameter Transmitters – ATEX/IECEx/UKCA	12
2.4	Ex instructions for M400 Series Multi-parameter Transmitters – FM Approval	14
2.4.1	Instructions of Use to Be Considered under FM Approval	14
2.4.1.1	General Notes	16
2.4.1.2	Cautionary Notes, Warnings and Markings	16
2.4.1.3	Control Drawings	18
3	Unit Overview	19
3.1	Overview ½ DIN	19
3.2	Control/Navigation Keys	20
3.2.1	Menu Structure	20
3.2.2	Navigation Keys	20
3.2.2.1	Navigating the Menu Tree	20
3.2.2.2	Escape	21
3.2.2.3	ENTER	21
3.2.2.4	Menu	21
3.2.2.5	Calibration Mode	21
3.2.2.6	Info Mode	21
3.2.3	Navigation of Data Entry Fields	21
3.2.4	Entry of Data Values, Selection of Data Entry Options	21
3.2.5	Navigation with ↑ in Display	22
3.2.6	"Save Changes" Dialog	22
3.2.7	Security Passwords	22
3.2.8	Display	22
4	Installation Instruction	23
4.1	Unpacking and Inspection of Equipment	23
4.1.1	Panel Cutout Dimensional Information – ½ DIN Models	23
4.1.2	Installation Procedure	24
4.1.3	Assembly – ½ DIN Version	24
4.1.4	½ DIN Version – Dimension Drawings	25
4.1.5	½ DIN Version – Pipe Mounting	25
4.2	Connection of Power Supply	26
4.2.1	Housing (Wall Mount)	26
4.3	Connector PIN Definition	27
4.3.1	Terminal Block (TB) Definitions	27
4.3.2	TB2 – Conductivity 4-e/2-e Analog Sensors	28
4.3.3	TB2 – pH/ORP Analog Sensors	28
4.3.4	TB2 – Oxygen Analog Sensors	29
4.3.5	TB2 – pH, Amp. Oxygen, Ozone, Conductivity 4-e and Dissolved CO ₂ (Low) ISM (Digital) Sensors	29
4.3.6	TB2 – Optical Oxygen, CO ₂ hi ISM (Digital) Sensors	30
4.4	Connection of ISM (Digital) Sensors	31
4.4.1	Connection of ISM Sensors for pH/ORP, Cond 4-e, Amp. Oxygen Measurement and Dissolved CO ₂ (Low)	31
4.4.2	TB2 – AK9 Cable Assignment	31
4.4.3	Connection of ISM Sensors for Optical Oxygen Measurement and CO ₂ hi (InPro 5500i)	32
4.5	Connection of Analog Sensors	33
4.5.1	Connection of Analog Sensor for pH/ORP	33
4.5.2	TB2 – Typical Wiring for Analog pH/ORP Sensor	34
4.5.2.1	Example 1	34
4.5.2.2	Example 2	35
4.5.2.3	Example 3	36
4.5.2.4	Example 4	37
4.5.3	Connection of Analog Sensor for Amperometric Oxygen Measurement	38
4.5.4	TB2 – Typical Wiring for Analog Sensor for Amperometric Oxygen Measurement	39
5	Placing Transmitter In, or Out, of Service	40
5.1	Placing Transmitter in Service	40
5.2	Placing Transmitter Out of Service	40
6	Quick Setup	41

7	Sensor Calibration	42
7.1	Enter Calibration Mode	42
7.1.1	Select the Desired Sensor Calibration Task	42
7.1.2	Finish Calibration	43
7.2	Conductivity Calibration for Two- or Four-Electrode Sensors	44
7.2.1	One-Point Sensor Calibration	45
7.2.2	Two-Point Sensor Calibration (Only for Four-Electrode Sensors)	46
7.2.3	Process Calibration	46
7.3	Calibration of Amperometric Oxygen Sensors	47
7.3.1	One-Point Calibration for Amperometric Oxygen Sensors	47
7.3.1.1	Auto Mode	48
7.3.1.2	Manual Mode	48
7.3.2	Process Calibration for Amperometric Oxygen Sensors	49
7.4	Calibration of Optical Oxygen Sensors (Only for ISM Sensors)	50
7.4.1	One-Point Calibration for Optical Oxygen Sensors	50
7.4.1.1	Auto Mode	50
7.4.1.2	Manual Mode	51
7.4.2	Two-Point Sensor Calibration	51
7.4.2.1	Auto Mode	52
7.4.2.2	Manual Mode	52
7.4.3	Process Calibration	53
7.5	pH Calibration	54
7.5.1	One-Point Calibration	54
7.5.1.1	Auto Mode	54
7.5.1.2	Manual Mode	55
7.5.2	Two-Point Calibration	55
7.5.2.1	Auto Mode	55
7.5.2.2	Manual Mode	56
7.5.3	Process Calibration	56
7.5.4	mV Calibration (Only for Analog Sensors)	57
7.5.5	ORP Calibration (Only for ISM Sensors)	58
7.6	Carbon Dioxide Calibration (Only for ISM Sensors)	58
7.6.1	One-Point Calibration	58
7.6.1.1	Auto Mode	59
7.6.1.2	Manual Mode	59
7.6.2	Two-Point Calibration	59
7.6.2.1	Auto Mode	60
7.6.2.2	Manual Mode	60
7.6.3	Process Calibration	61
7.7	Calibration of Ozone Sensors (Only ISM Sensors)	61
7.7.1	One-Point ZeroPt Calibration for Ozone Sensors	61
7.7.2	Process Calibration for Ozone Sensors	62
7.8	Sensor Temperature Calibration (Only for Analog Sensors)	63
7.8.1	One-Point Sensor Temperature Calibration	63
7.8.2	Two-Point Sensor Temperature Calibration	63
7.9	Edit Sensor Calibration Constants (Only for Analog Sensors)	64
7.10	Sensor Verification	64
8	Configuration	65
8.1	Enter Configuration Mode	65
8.2	Measurement	65
8.2.1	Channel Setup	65
8.2.1.1	Analog Sensor	66
8.2.1.2	ISM Sensor	66
8.2.1.3	Save Changes of the Channel Setup	67
8.2.2	Temperature Source (Only for Analog Sensors)	67
8.2.3	Parameter Related Settings	68
8.2.3.1	Conductivity Temperature Compensation	68
8.2.3.2	Concentration Table	69
8.2.3.3	pH/ORP Parameters	71
8.2.3.4	Parameters for Oxygen Measurement Based on Amperometric Sensors	72
8.2.3.5	Parameters for Oxygen Measurement Based on Optical Sensors	73
8.2.3.6	Adjusting Sampling Rate for Optical Sensors	74
8.2.3.7	LED Mode	74
8.2.3.8	Dissolved Carbon Dioxide Parameters	75
8.2.3.9	Thermal Conductivity Dissolved Carbon Dioxide Parameters	76
8.2.4	Self Averaging	77

8.3	Alarm/Clean	77
8.3.1	Alarm	78
8.3.2	Clean	79
8.4	ISM Set Up (Available for pH, Oxygen and Dissolved Carbon Dioxid ISM Sensors)	80
8.4.1	Sensor Monitoring	80
8.4.2	CIP Cycle Limit	82
8.4.3	SIP Cycle Limit	82
8.4.4	Autoclaving Cycle Limit	83
8.4.5	Reset ISM Counter/Timer	84
8.4.6	DLI Stress Adjustment (Only for pH ISM Sensors)	84
8.5	Display	85
8.5.1	Measurement	85
8.5.2	Resolution	85
8.5.3	Backlight	86
8.5.4	Name	86
8.5.5	ISM Sensor Monitoring (Available When ISM Sensor Connected)	86
8.6	Hold Outputs	87
9	System	88
9.1	Set Language	88
9.2	Passwords	88
9.2.1	Changing Passwords	89
9.2.2	Configuring Menu Access for Operator	89
9.3	Set/Clear Lockout	89
9.4	Reset	90
9.4.1	Reset System	90
9.4.2	Reset Meter Calibration	90
9.5	Set Date & Time	90
10	Service	91
10.1	Diagnostics	91
10.1.1	Model/Software Revision	91
10.1.2	Display	91
10.1.3	Keypad	92
10.1.4	Memory	92
10.1.5	Read Analog Inputs	92
10.1.6	O ₂ Optical	92
10.2	Calibrate	93
10.2.1	Calibrate Meter (Only for Channel A)	93
10.2.1.1	Resistance	93
10.2.1.2	Temperature	94
10.2.1.3	Current	95
10.2.1.4	Voltage	96
10.2.1.5	Rg Diagnostic	96
10.2.1.6	Rr Diagnostic	97
10.2.1.7	Calibrate Analog Input Signal	97
10.2.2	Calibrate Unlock	98
10.3	Tech Service	98
11	Info	99
11.1	Messages	99
11.2	Calibration Data	99
11.3	Model/Software Revision	100
11.4	ISM Sensor Info (Available when ISM Sensor Connected)	100
11.5	ISM Sensor Diagnostics (Available when ISM Sensor Connected)	100
12	PROFIBUS PA Interface	103
12.1	General	103
12.1.1	System Architecture	103
12.2	M400 PA Block Model	104
12.2.1	Block Configuration	105
12.3	Commissioning	106
12.3.1	Network Configuration	106
12.3.2	Set PROFIBUS address	106
12.3.3	Device Master File (GSD file)	106
13	Maintenance	108
13.1	Front Panel Cleaning	108

14	Troubleshooting	109
14.1	Cond (resistive) Error Messages/Warning- and Alarm List for Analog Sensors	109
14.2	Cond (resistive) Error Messages/Warning- and Alarm List for ISM Sensors	110
14.3	pH Error Messages/Warning- and Alarm List	110
14.3.1	pH Sensors except Dual Membrane pH Electrodes	110
14.3.2	Dual Membrane pH Electrodes (pH/pNa)	111
14.3.3	ORP Messages	111
14.4	Amperometric O ₂ Error Messages/Warning- and Alarm List	112
14.4.1	High Level Oxygen Sensors	112
14.4.2	Low Level Oxygen Sensors	112
14.4.3	Trace Oxygen Sensors	113
14.5	Optical O ₂ Error Messages/Warning- and Alarm List	113
14.6	Dissolved Carbon Dioxide Error Messages/Warning- and Alarm List	114
14.7	Thermal conductivity CO ₂ sensor/Warning- and alarm messages	114
14.8	Warning- and Alarm Indication on the Display	115
14.8.1	Warning Indication	115
14.8.2	Alarm Indication	115
15	Accessories and Spare Parts	116
16	Specifications	117
16.1	General Specifications	117
16.2	Electrical Specifications	121
16.3	PROFIBUS PA Interface Specification	121
16.4	Mechanical Specification	121
16.5	Environmental Specifications	122
16.6	Control Drawings	123
16.6.1	Installation, Maintenance and Inspection	123
16.6.2	Control Installation Drawing General Installation	124
16.6.3	Notes	127
17	Default Table	128
18	Warranty	133
19	Buffer Tables	134
19.1	Standard pH Buffers	134
19.1.1	Mettler-9	134
19.1.2	Mettler-10	135
19.1.3	NIST Technical Buffers	135
19.1.4	NIST Standard Buffers (DIN and JIS 19266: 2000–01)	136
19.1.5	Hach Buffers	136
19.1.6	Ciba (94) Buffers	137
19.1.7	Merck Titrisole, Riedel-de-Haën Fixanale	137
19.1.8	WTW Buffers	138
19.1.9	JIS Z 8802 Buffers	138
19.2	Dual Membrane pH Electrode Buffers	139
19.2.1	Mettler-pH/pNa Buffers (Na+ 3.9M)	139

1 Introduction

1.1 Intended Use

The M400 PA multi-parameter transmitter is a single channel online process instrument with PROFIBUS® communication capabilities for measuring various properties of fluids and gases. The transmitter is able to measure following parameters: pH/ORP, Oxygen, Dissolved Carbon Dioxide, Conductivity and Ozone.

The M400 PA is a mixed mode transmitter able to handle analog or ISM™ (digital) sensors.

M400 PA parameter fit guide

Parameter	M400 PA	
	Analog	ISM
pH/ORP	•	•
pH/pNa	–	•
Conductivity 2-e	•	–
Conductivity 4-e	•	•
Amp. DO ppm/ppb/trace	•/•/•	•/•/•
Amp. O ₂	•	•
Optical Oxygen ppm/ppb	–	•/•
Ozone		
Dissolved Carbon Dioxide (low)	–	•
CO ₂ hi (InPro 5500i)	–	•

A large four line backlit Liquid Crystal Display conveys measuring data and setup information. The menu structure allows the operator to modify all operational parameters by using keys on the front panel. A menu-lockout feature, with password protection, is available to prevent the unauthorized use of the meter. Via the PROFIBUS PA interface the Analog Output Block, Discrete Input Block and Discrete Output Block can be configured for Alarm/Clean status, Hold status and pressure compensation.

This description corresponds to the firmware release, version V1.0.0 for transmitter M400 PA. Changes are taking place constantly, without prior notification.

2 Safety Instructions

This manual includes safety information with the following designations and formats.

2.1 Definition of Equipment and Documentation Symbols and Designations



WARNING: POTENTIAL FOR PERSONAL INJURY.



CAUTION: possible instrument damage or malfunction.



NOTE: Important operating information.



On the transmitter or in this manual text indicates: Caution and/or other possible hazard including risk of electric shock (refer to accompanying documents)

The following is a list of general safety instructions and warnings. Failure to adhere to these instructions can result in damage to the equipment and/or personal injury to the operator.

- The M400 Transmitter should be installed and operated only by personnel familiar with the transmitter and who are qualified for such work.
- The M400 Transmitter must only be operated under the specified operating conditions (see section 16 “Specifications”).
- Repair of the M400 Transmitter must be performed by authorized, trained personnel only.
- With the exception of routine maintenance, cleaning procedures or fuse replacement, as described in this manual, the M400 Transmitter must not be tampered with or altered in any manner.
- METTLER TOLEDO accepts no responsibility for damage caused by unauthorized modifications to the transmitter.
- Follow all warnings, cautions, and instructions indicated on and supplied with this product.
- Install equipment as specified in this instruction manual. Follow appropriate local and national codes.
- Protective covers must be in place at all times during normal operation.
- If this equipment is used in a manner not specified by the manufacturer, the protection provided by it against hazards may be impaired.



WARNINGS:

Installation of cable connections and servicing of this product require access to shock hazard voltage levels.

Main power wired to separate power source must be disconnected before servicing.

Switch or circuit breaker shall be in close proximity to the equipment and within easy reach of the OPERATOR; it shall be marked as the disconnecting device for the equipment. Main power must employ a switch or circuit breaker as the disconnecting device for the equipment.

Electrical installation must be in accordance with the National Electrical Code and/or any other applicable national or local codes.



NOTE: PROCESS UPSETS Because process and safety conditions may depend on consistent operation of this transmitter, provide appropriate means to maintain operation during sensor cleaning, replacement or sensor or instrument calibration.

2.2 Environmental protection



Waste electrical products should not be disposed of with household waste. Please recycle where facilities exist. Check with your Local Authority or retailer for recycling advice.



2.3 Ex Instructions for M400 Series Multi-parameter Transmitters – ATEX/IECEX/UKCA

M400 series multi-parameter transmitters are produced by Mettler-Toledo GmbH. It has passed the inspection of IECEX and conforms to following standards:

- **IEC 60079-0 : 2017**
Edition: 7.0 Explosive atmospheres –
Part 0: General requirements
- **IEC 60079-11 : 2011**
Edition: 6.0 Explosive atmospheres –
Part 11: Equipment protection by intrinsic safety “i”

Ex Marking:

- **Ex ib [ia Ga] IIC T4 Gb**
- **Ex ib [ia Da] IIIC T80 °C Db IP66**

Certificate No.:

- **IECEX NEP 18.0007X**
- **SEV 12 ATEX 0132X**
- **CML 22 UKEX 2209X**

1. Special Conditions of use (X-marking in the Certificate Number):


1. Avoid ignition hazard due to impact or friction, prevent mechanical sparks.
2. Avoid electrostatic discharge on enclosure surface, use wet cloth only for cleaning.
3. In hazardous area, IP66 cable glands (as supplied) must be mounted.

2. Pay particular attention to the following when using the transmitter:

1. Rated ambient temperature range:
 - for gas atmosphere: –20 ~ +60 °C
 - for dust atmosphere: –20 ~ +57 °C
2. No operation on the upgrade interface in hazardous area.
3. Users shall not arbitrarily replace the internal electrical components.
4. When installation, use and maintenance, IEC 60079-14 should be observed.
5. When installation in explosive dust atmosphere
 - 5.1 Cable gland or blanking plug to IEC 60079-0:2017 and IEC 60079-11: 2011 with marking Ex ai IIIC IP66 should be adopted.
 - 5.2 The overlay switch of multi-parameter transmitter shall be protected from light.
 - 5.3 Avoid high risk of mechanical danger on the overlay switch.
6. Observe the warning: potential electrostatic charging hazard- see instructions, avoid ignition hazard due to impact or friction for Ga application.
7. For connection to intrinsically safe circuits, use the maximum values in the following table.

Terminal	Function	Safety Parameters				
10, 11	Power (PA) FISCO field device	$U_i = 17.5\text{ V}$	$I_i = 380\text{ mA}$	$P_i = 5.32\text{ W}$	$L_i = 0$	$C_i = 3\text{ nF}$
	Linear power	$U_i = 24\text{ V}$	$I_i = 200\text{ mA}$	$P_i = 1.2\text{ W}$	$L_i = 0$	$C_i = 3\text{ nF}$
P, Q	Analog input	$U_i = 24\text{ V}$	$I_i = 100\text{ mA}$	$P_i = 0.8\text{ W}$	$L_i = 0$	$C_i = 15\text{ nF}$
N, O	RS485 sensor	$U_o = 5.88\text{ V}$ $U_i = 24\text{ V}$	$I_o = 54\text{ mA}$ $I_i = 100\text{ mA}$	$P_o = 79\text{ mW}$ $P_i = 0.8\text{ W}$	$L_o = 1\text{ mH}$ $L_i = 0$	$C_o = 1.9\text{ }\mu\text{F}$ $C_i = 0.7\text{ }\mu\text{F}$
L, M	One-wire sensor	$U_o = 5.88\text{ V}$	$I_o = 22\text{ mA}$	$P_o = 32\text{ mW}$	$L_o = 1\text{ mH}$	$C_o = 2.8\text{ }\mu\text{F}$
I, J, K	Temperature sensor	$U_o = 5.88\text{ V}$	$I_o = 5.4\text{ mA}$	$P_o = 8\text{ mW}$	$L_o = 5\text{ mH}$	$C_o = 2\text{ }\mu\text{F}$
B, C, D, H	Dissolved oxygen sensor	$U_o = 5.88\text{ V}$	$I_o = 29\text{ mA}$	$P_o = 43\text{ mW}$	$L_o = 1\text{ mH}$	$C_o = 2.5\text{ }\mu\text{F}$
A, B, E, G	Conductivity sensor	$U_o = 5.88\text{ V}$	$I_o = 29\text{ mA}$	$P_o = 43\text{ mW}$	$L_o = 1\text{ mH}$	$C_o = 2.5\text{ }\mu\text{F}$
A, E, G	pH sensor	$U_o = 5.88\text{ V}$	$I_o = 1.3\text{ mA}$	$P_o = 1.9\text{ mW}$	$L_o = 5\text{ mH}$	$C_o = 2.1\text{ }\mu\text{F}$

MODEL: M400/2XH
 Feeding Voltage: 14 to 30 VDC
 $T_{[amb]}$: -20 to +60 °C (Gas)
 -20 to +57 °C (Dust)



P/N: S/N:

CE 1258 **UK CA** 2503 **METTLER TOLEDO**
 www.mt.com/pro
 Mettler-Toledo GmbH
 Im Hackacker 15
 8902 Urdorf, Switzerland

Ex **IECEX**
 II(1) G Ex ib[ia Ga] IIC T4 Gb
 II(1) D Ex ib[ia Da] IIIC T80°C Db IP66
 SEV 12 ATEX 0132 X
 IECEx NEP 18 0007X
 CML 22 UKEX 2209X
 Electrical data see user manual Made by METTLER TOLEDO in China

Label M400 PA.

2.4 Ex instructions for M400 Series Multi-parameter Transmitters – FM Approval

2.4.1 Instructions of Use to Be Considered under FM Approval



M400 series multi-parameter transmitters are produced by Mettler-Toledo GmbH. It has passed the inspection of NRTL cFMus and to following requirements:

The equipment is provided with an internal bond wiring and an internal flying lead wire for grounding purposes.

US marking	
Operating temperature range	–20 °C to +60 °C (–4 °F to +140 °F)
Environmental designation	Enclosure type 4X, IP66
Intrinsically safe	– Class I, Division 1, Groups A, B, C, D T4A – Class II, Division 1, Groups E, F, G – Class III
Intrinsically safe	Class I, Zone 0, AEx ia IIC T4 Ga
Parameters	– Entify: Control drawing 12112601 and 12112602 – FISCO: Control drawing 12112603 and 12112602
Nonincendive	– Class I, Division 2, Groups A, B, C, D T4A – Class I, Zone 2, Groups IIC T4
Certificate no.	3046275
Standards	– FM3810:2005 Approval Standard for Electrical Equipment for Measurement, Control and Laboratory Use – ANSI/IEC-60529:2004 Degrees of Protection Provided by Enclosures (IP Codes) – ANSI/ISA-61010-1:2004 Edition: 3.0 Safety Requirements for Electrical Equipment for Measurement, Control, and Laboratory Use – Part 1: General Requirements – ANSI/NEMA 250:1991 Enclosures for Electrical Equipment (1,000 Volts Maximum) – FM3600:2011 Approval Standard for Electrical Equipment for Use in Hazardous (Classified) Locations – General Requirements – FM3610:2010 Approval Standard for Intrinsically Safe Apparatus and Associated Apparatus for Use in Class I, II & III, Division 1, Hazardous (Classified) Locations – FM3611:2004 Approval Standard for Nonincendive Electrical Equipment for Use in Class I & II, Division 2, and Class III, Division 1 & 2, Hazardous (Classified) Locations – ANSI/ISA-60079-0:2013 Edition: 6.0 Explosive Atmospheres – Part 0: General Requirements – ANSI/ISA-60079-11:2012 Edition: 6.0 Explosive Atmospheres – Part 11: Equipment Protection by Intrinsic Safety “i”

Canadian marking	
Operating temperature range	–20 °C to +60 °C (–4 °F to +140 °F)
Environmental designation	Enclosure type 4X, IP66
Intrinsically safe	– Class I, Division 1, Groups A, B, C, D T4A – Class II, Division 1, Groups E, F, G – Class III
Intrinsically safe	Class I, Zone 0, Ex ia IIC T4 Ga
Parameters	– Entity: Control drawing 12112601 and 12112602 – FISCO: Control drawing 12112603 and 12112602
Nonincendive	Class I, Division 2, Groups A, B, C, D T4A
Certificate no.	3046275
Standards	– CAN/CSA-C22.2 No. 60529:2010 Degrees of Protection Provided by Enclosures (IP Codes) – CAN/CSA-C22.2 No. 61010-1:2004 Edition: 3.0 Safety Requirements for Electrical Equipment for Measurement, Control, and Laboratory Use – Part 1: General Requirements – CAN/CSA-C22.2 No. 94:1976 Special Purpose Enclosures – Industrial Products – CAN/CSA-C22.2 No. 213-M1987:2013 Non-Incendive Equipment for Use in Class I, Division 2 Hazardous Locations – Industrial Products – CAN/CSA-C22.2 No. 60079-0:2011 Edition: 2.0 Explosive Atmospheres – Part 0: General Requirements – CAN/CSA-C22.2 No. 60079-11:2014 Edition: 2.0 Explosive Atmospheres – Part 11: Equipment Protection by Intrinsic Safety “i”

2.4.1.1 General Notes

The Multi-parameter Transmitter M400/2(X)H, M400G/2XH, M400FF, M400PA are suitable for use in hazardous atmospheres of all combustible materials of explosion groups A, B, C, D, E, F and G for applications requiring Class I, II, III, Division 1 instruments and groups A, B, C and D for applications requiring Class I, Division 2 instruments (National Electrical Code® (ANSI/NFPA 70 (NEC®), Article 500; or Canadian Electrical (CE) Code® (CEC Part 1, CAN/CSA-C22.1), Appendix F when installed in Canada), or of explosion groups IIC, IIB or IIA for applications requiring Class I, Zone O, AEx/Ex ia IIC T4, Ga instruments (National Electrical Code® (ANSI/NFPA 70 (NEC®), Article 500; or Canadian Electrical (CE) Code® (CEC Part 1, CAN/CSA-C22.1), Appendix F when installed in Canada).

If the Multi-parameter Transmitter M400/2(X)H, M400G/2XH, M400FF, M400PA is installed and operated in hazardous areas, the general Ex installation regulations as well as these safety instructions must be observed.

The operating instructions as well as the installation regulations and standards that apply for explosion protection of electrical systems must always be observed.

The installation of explosion-endangered systems must always be carried out by qualified personnel.

For mounting instructions on specific valves refer to the mounting instructions supplied with the mounting kit. Mounting does not affect the suitability of the SVI FF positioner for use in a potentially hazardous environment.

The equipment is not intended to be used as personal protective equipment. To prevent injury, read the manual before use.

For language translation assistance contact your local representative or email process.service@mt.com.

Pour la langue de traduction aide, contactez votre représentant local ou envoyez un e-mail process.service@mt.com.

2.4.1.2 Cautionary Notes, Warnings and Markings

Hazardous location notes:

1. For guidance on US installations, see ANSI/ISA-RP12.06.01, Installation of Intrinsically Safe Systems for Hazardous (Classified) Locations.
2. Installations in the US shall comply with the relevant requirements of the National Electrical Code® (ANSI/NFPA 70 (NEC®)).
3. Installations in Canada shall comply with the relevant requirements of the Canadian Electrical (CE) Code® (CEC Part 1, CAN/CSA-C22.1).
4. Wiring methods must conform to all local and national codes governing the installation, and wiring must be rated for at least +10 °C above the highest expected ambient temperature.
5. Where the protection type allows and depends on wiring glands, the glands must be certified for the type of protection required and area classification identified on the equipment or system nameplate.
6. The internal grounding terminal shall be used as the primary equipment grounding means and the external grounding terminal is only for a supplemental (secondary) bonding connection where local authorities permit or require such a connection.

7. A dust-tight conduit seal shall be used when installed in Class II conductive and non-conductive dust environments and Class III combustible flying environments.
8. Approved seals against ingress of water or dust are required and the NPT or metric thread fittings must be sealed with tape or thread sealant in order to meet the highest level of ingress protection.
9. When the equipment is supplied with plastic dust plugs in the conduit/cable gland entries; it is the end-user's responsibility to provide cable glands, adaptors and/or blanking plugs suitable for the environment in which the equipment is installed. When installed in a hazardous (classified) location, the cable glands, adaptors and/or blanking plugs shall additionally be suitable for the hazardous (classified) location, the product certification, and acceptable to the local authority having jurisdiction for the installation.
10. The end-user must consult the manufacturer for repair disclaimers, and only certified parts, such as entry plugs, mounting and cover lock screws and gaskets, supplied by the manufacturer are permitted. No substitutions with non-manufacturer supplied parts are permitted.
11. Tighten cover screws to 1.8 Nm (15.8 lb-in.). Overtorquing may cause enclosure breakage.
12. The minimum tightening torque for M4 (No. 6) binding screw protective conductor terminals is 1.2 Nm (10.6 lb-in.) or greater, as specified.
13. Care must be taken during installation to avoid impacts or friction that could create an ignition source.
14. Use copper, copper-clad aluminum or aluminum conductors only.
15. The recommended tightening torque for field wiring terminals is 0.8 Nm (7 lb-in.) or greater, as specified.
16. The Nonincendive version of the Multi-parameter Transmitter M400/2H must be connected to limited output NEC Class 2 circuits, as outlined in the National Electrical Code® (ANSI/NFPA 70 (NEC®)), only. If the devices are connected to a redundant power supply (two separate power supplies), both must meet this requirement.
17. The Class I, Zone 2 certifications are based on Division evaluations and the marking acceptance of Article 505 of the National Electrical Code® (ANSI/NFPA 70 (NEC®)).
18. The Multi-parameter Transmitter M400/2(X)H, M400G/2XH, M400FF, M400PA assessed were certified by FM Approvals under a Type 3 Certification System as identified in ISO Guide 67.
19. Tampering and replacement with non-factory components may adversely affect the safe use of the system.
20. Insertion or withdrawal of removable electrical connectors is to be accomplished only when the area is known to be free of flammable vapors.
21. The Multi-parameter Transmitter M400/2(X)H, M400G/2XH, M400FF, M400PA is not intended for servicing or maintenance operation. Malfunctioning units operating out of manufacturer's specification should be discarded and replaced with a new operational unit.
22. Substitution of components may impair intrinsic safety.
23. Do not open when an explosive atmosphere is present.
24. Explosion hazard, do not disconnect while circuit is live unless area is known to be non-hazardous.
25. Explosion hazard, substitution of components may impair suitability for Class I, Division 2.

The Multi-parameter Transmitter M400 FF, M400 PA intrinsically safe apparatus, entity/fieldbus intrinsically safe concept version, bears the following label marking:



Label Model M400 PA.


2.4.1.3 Control Drawings

Refer to section „16.6 Control Drawings“ auf Seite 123.


3 Unit Overview

The M400 models are available in ½ DIN case size. The M400 models provide an integral IP66/NEMA4X housing for wall- or pipe mount.

3.1 Overview ½ DIN

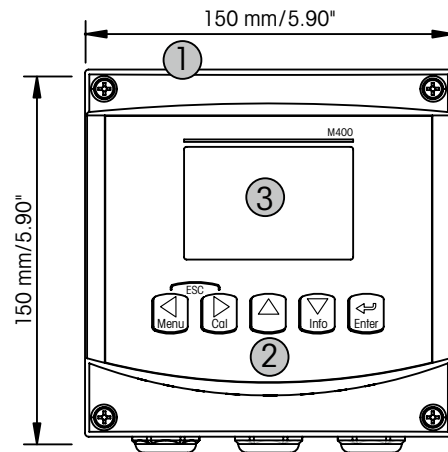

- 1: Hard Polycarbonate Case
- 2: Five Tactile-Feedback Navigation Keys
- 3: Four-line LC Display

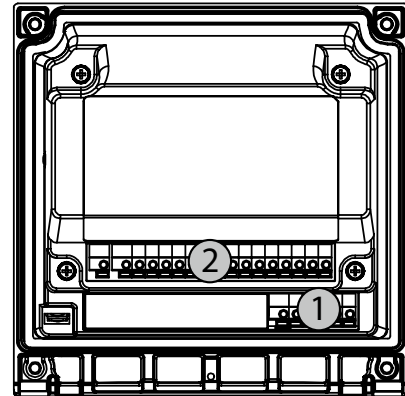


- 1: TB1 – PA
- 2: TB2 – Sensor Signal

3.2 Control/Navigation Keys

3.2.1 Menu Structure

Below is the structure of the M400 menu tree:

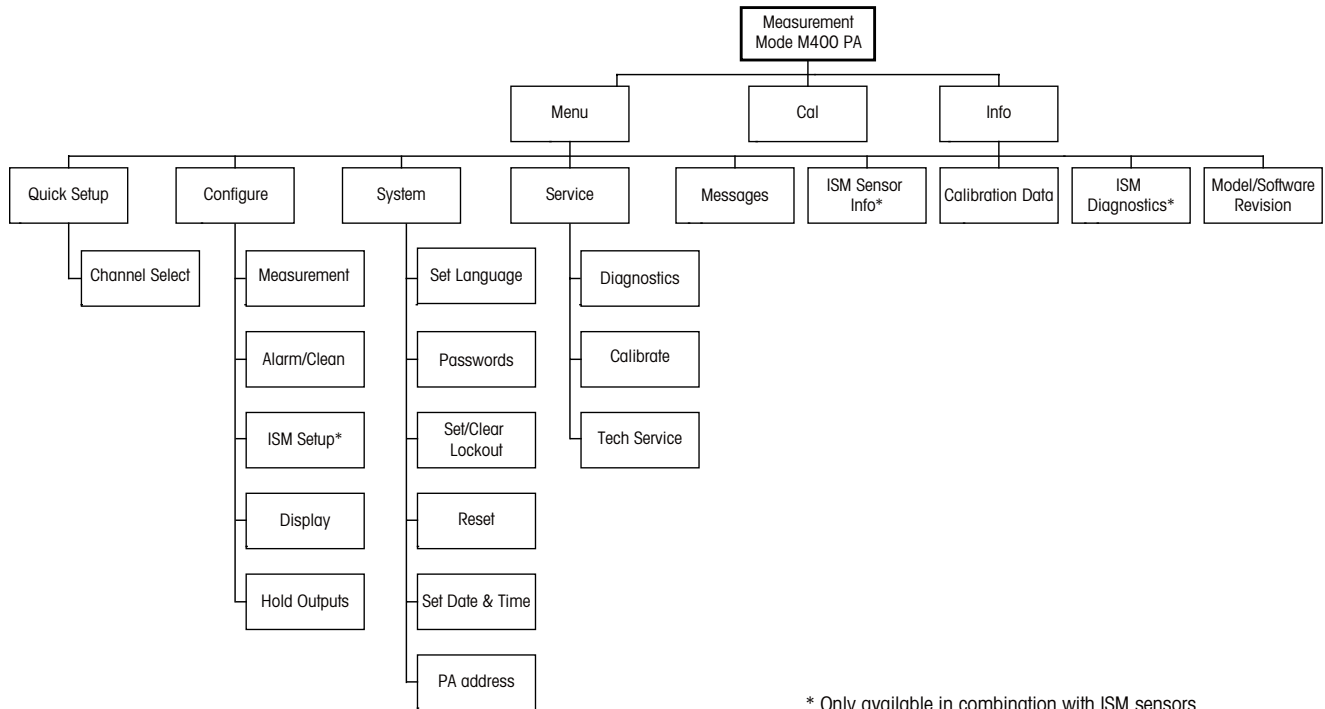

* Only available in combination with ISM sensors

3.2.2 Navigation Keys



3.2.2.1 Navigating the Menu Tree

Enter the desired main Menu branch with the ◀▶ or ▲ keys. Use the ▲ and ▼ keys to navigate through the selected Menu branch.



NOTE: In order to back up one menu page, without escaping to the measurement mode, move the cursor under the UP Arrow character (↑) at the bottom right of the display screen and press [ENTER].

3.2.2.2 Escape

Press the ◀ and ▶ key simultaneously (escape) to return to the Measurement mode.

3.2.2.3 ENTER

Use the ↵ key to confirm action or selections.

3.2.2.4 Menu

Press the ◀ key to access the main Menu.

3.2.2.5 Calibration Mode

Press the ▶ key to enter Calibration mode.

3.2.2.6 Info Mode

Press the ▼ key to enter Info mode.

3.2.3 Navigation of Data Entry Fields

Use the ▶ key to navigate forward or the ◀ key to navigate backwards within the changeable data entry fields of the display.

3.2.4 Entry of Data Values, Selection of Data Entry Options

Use the ▲ key to increase or the ▼ key to decrease a digit. Use the same keys to navigate within a selection of values or options of a data entry field.



NOTE: Some screens require configuring multiple values via the same data field. Be sure to use the ▶ or ◀ key to return to the primary field and the ▲ or ▼ key to toggle between all configuration options before entering to the next display screen.

3.2.5 Navigation with ↑ in Display

If a ↑ is displayed on the bottom right hand corner of the display, you can use the ► or the ◀ key to navigate to it. If you click [ENTER] you will navigate backwards through the menu (go back one screen). This can be a very useful option to move back up the menu tree without having to exit into the measuring mode and re-enter the menu.

3.2.6 "Save Changes" Dialog

Three options are possible for the "Save changes" dialog: Yes & Exit (Save changes and exit to measuring mode), "Yes & ↑" (Save changes and go back one screen) and "No & Exit" (Don't save changes and exit to measuring mode). The "Yes & ↑" option is very useful if you want to continue configuring without having to re-enter the menu.

3.2.7 Security Passwords

The M400 transmitter allows a security lock-out of various menus. If the security lock-out feature of the transmitter has been enabled, a security password must be entered to allow access to the menu. See section 9.3 "Set/Clear Lockout" for more information.

3.2.8 Display



NOTE: In the event of an alarm or other error condition the M400 Transmitter will display a flashing Δ in the upper right corner of the display. This symbol will remain until the condition that caused it has been cleared.



NOTE: Channel A indicates that an analog sensor is connected to the transmitter. Channel B indicates, that an ISM (digital) sensor is connected to the transmitter.



NOTE: During calibration of an analog sensor a flashing "H" (Hold) appears in the upper left corner of the display. During calibration of an ISM sensor a flashing "H" (Hold) appears. This symbol will remain for 20 sec., after end of calibration. This symbol will remain for 20 seconds until after the calibration or clean is completed. This symbol will also disappear when Digital In is deactivated.

The M400 is a single input channel transmitter, and only one sensor can be connected at the same time.

4 Installation Instruction

4.1 Unpacking and Inspection of Equipment

Inspect the shipping container. If it is damaged, contact the shipper immediately for instructions. Do not discard the box.

If there is no apparent damage, unpack the container. Be sure all items shown on the packing list are present.


If items are missing, notify METTLER TOLEDO immediately.

4.1.1 Panel Cutout Dimensional Information – ½ DIN Models

½ DIN Model transmitters are designed with an integral rear cover for stand-alone wall mount installation.

The unit may also be wall mounted using the integral rear cover. See installation instructions in section 4.1.2 "Installation Procedure".

Below are cut-out dimensions required by the ½ DIN models when mounted within a flat panel or on a flat enclosure door. This surface must be flat and smooth. Textured or rough surfaces are not recommended and may limit the effectiveness of the gasket seal provided.

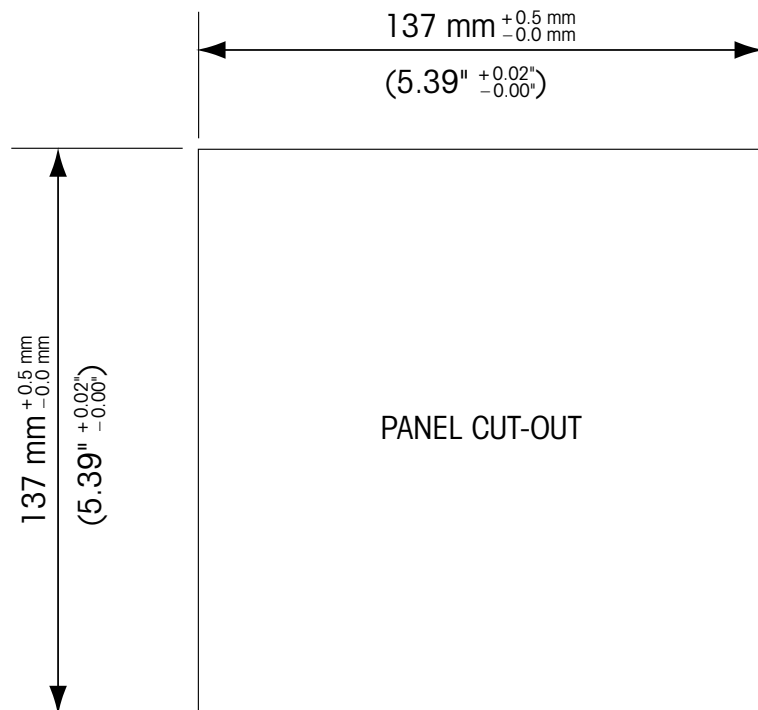

Optional hardware accessories are available that allow for panel- or pipe-mount. Refer to section 15 "Accessories and Spare Parts" for ordering information.

4.1.2 Installation Procedure

General:

- Orient the transmitter so that the cable grips face downward.
- Wiring routed through the cable grips shall be suitable for use in wet locations.
- In order provide IP66 enclosure ratings, all cable glands must be in place. Each cable gland must be filled using a cable, or suitable Cable Gland Hole Seal.


For Wall Mount:

- Remove rear cover from front housing.
- Start by unscrewing the four screws located on the face of the transmitter, in each corner. This allows the front cover to swing away from the rear housing.
- Remove the hinge-pin by squeezing the pin from each end. This allows the front housing to be removed from the rear housing.
- Mount rear housing to wall. Secure mounting kit to the M400 according to the supplied instructions. Attach to wall using appropriate mounting hardware for wall surface. Be sure it is level and securely fastened and the installation adheres to any and all clearance dimensions required for transmitter service and maintenance. Orient the transmitter so that the cable grips are facing downward.
- Replace the front housing to the rear housing. Securely tighten the rear-cover screws to ensure that IP66/NEMA4X enclosure environmental rating is maintained. The unit is ready to be wired.

For Pipe Mount:


- Use only manufacturer-supplied components for pipe-mounting the M400 transmitter and install per the supplied instructions. See section 15 "Accessories and Spare Parts" for ordering information.

4.1.3 Assembly – ½ DIN Version

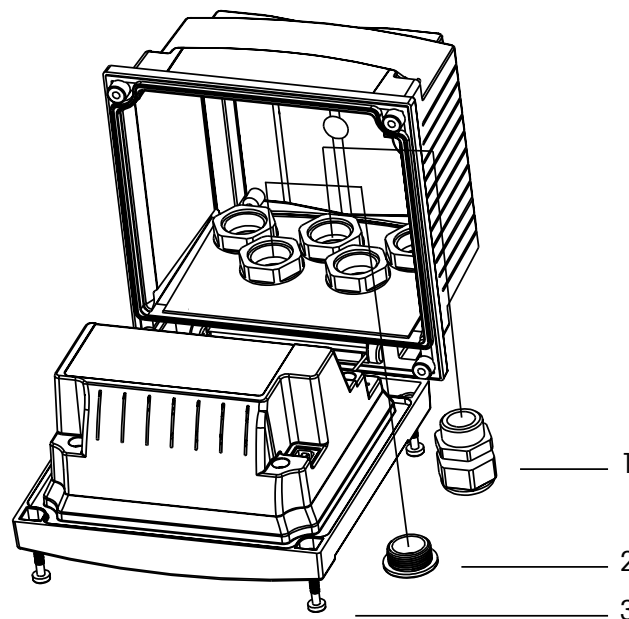


1. 5 pieces M20X1.5 cable glands
2. 2 pieces plastics plugs
3. 3 pieces screws

4.1.4 ½ DIN Version – Dimension Drawings

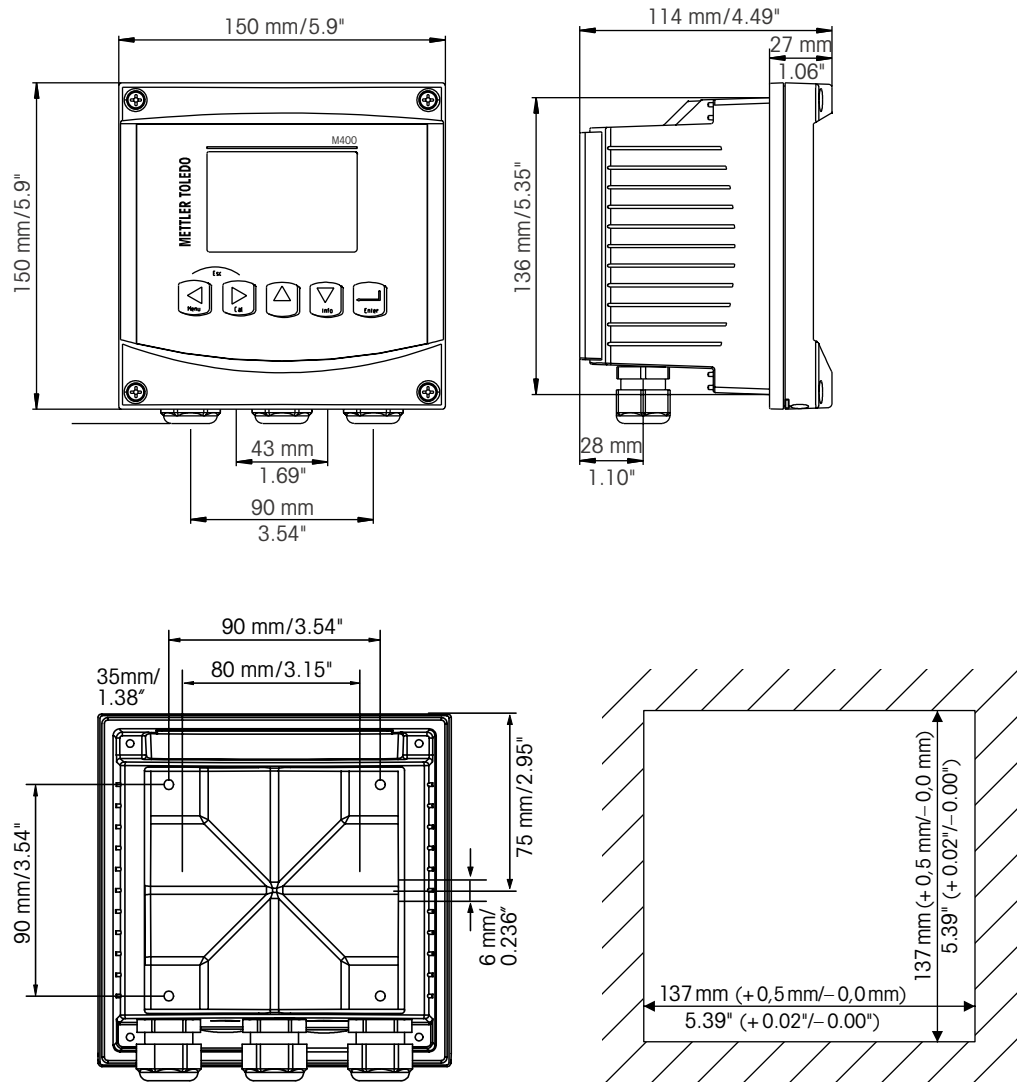

4.1.5 ½ DIN Version – Pipe Mounting

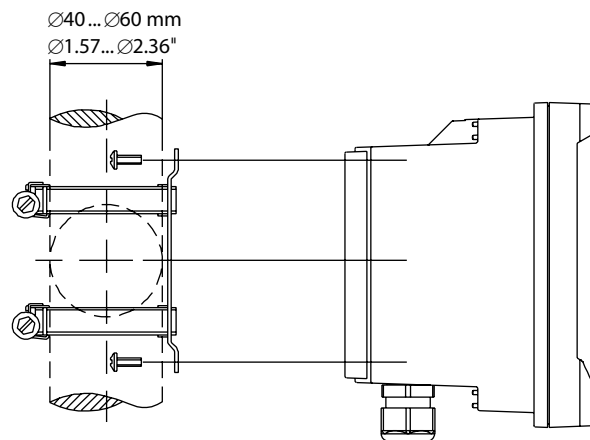

4.2 Connection of Power Supply


All connections to the transmitter are made on the rear panel of all models.



Be sure power to all wires is turned off before proceeding with the installation.


A two-terminal connector on the rear panel of all M400 models is provided for power connection. All M400 PA models are designed to operate in non-hazardous area from a 9 to 32 V DC power source (linear barrier: 9 to 24 V DC). Refer to specifications for power requirements and ratings and size power wiring accordingly (AWG 16 – 24, wire cross-section 0.2 mm² to 1.5 mm²).

The terminal block for power connections is labeled "PROFIBUS PA" on the rear panel of the transmitter. Connect the transmitter to the **–PROFIBUS PA** and **+PROFIBUS PA** terminals.

The terminals are suitable for single wires and flexible leads 0.2 mm² to 2.5 mm² (AWG 16 – 24). –PROFIBUS PA and +PROFIBUS PA terminals are available twice. There is no earth ground terminal on the transmitter. For this reason the internal power wiring within the transmitter is double insulated and the product label designates this using the  symbol.

For further information e. g. on the cable specifications, see PNO-Richtlinie 2.092 PROFIBUS PA "User and Installation Guideline" and IEC 61158-2 (MBP).


4.2.1 Housing (Wall Mount)

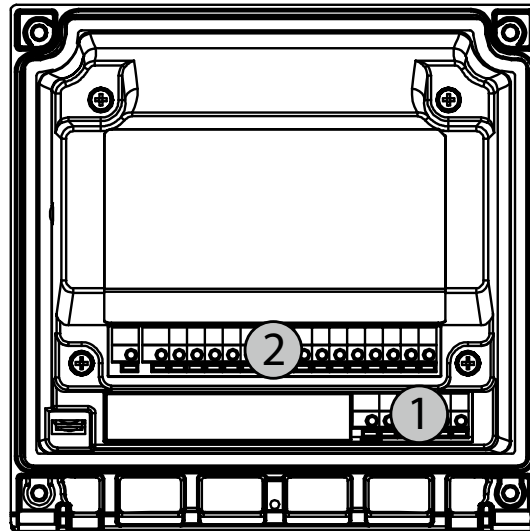

- 1: TB1 – PROFIBUS PA
- 2: TB2 – Sensor Signal

4.3 Connector PIN Definition

4.3.1 Terminal Block (TB) Definitions

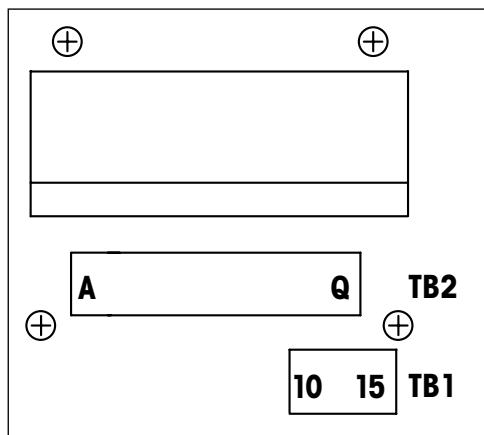

Power connections are labeled +PROFIBUS PA and –PROFIBUS PA for non-hazardous area: 9 to 32 V DC

TB1

1	Not available
2	Not available
3	Not available
4	Not available
5	Not available
6	Not available
7	Not available
8	Not available
9	Not available
10	+PROFIBUS PA
11	–PROFIBUS PA
12	+PROFIBUS PA
13	–PROFIBUS PA
14	Not used
15	⏏

4.3.2 TB2 – Conductivity 4-e/2-e Analog Sensors

TB2 – Analog Sensors

	Cond 4-e or 2-e	
Terminal	Function	Color
A	Cnd inner1*	white
B	Cnd outer1*	white/blue
C	Cnd outer1	–
D	Not used	–
E	Cnd outer2	–
F	Cnd inner2**	blue
G	Cnd outer2 (GND)**	black
H	Not used	–
I	RTD ref/GND	bare shield
J	RTD sense	red
K	RTD	green
L	Not used	–
M	Not used	–
N	Not used	–
O	Not used	–
P	Not used	–
Q	Not used	–

* For third party Cond 2-e sensors a jumper between A and C may be required.

** For third party Cond 2-e sensors a jumper between F and G may be required.

4.3.3 TB2 – pH/ORP Analog Sensors

TB2 – Analog Sensors

	pH		Redox (ORP)	
Terminal	Function	Color*	Function	Color
A	Glass	transparent	Platinum	transparent
B	Not used	–	–	–
C	Not used	–	–	–
D	Not used	–	–	–
E	Reference	red	Reference	red
F	Reference**	–	Reference**	–
G	Solution GND**	blue***	Solution GND**	–
H	Not used	–	–	–
I	RTD ref/GND	white	–	–
J	RTD sense	–	–	–
K	RTD	green	–	–
L	Not used	–	–	–
M	Shield (GND)	green/yellow	Shield (GND)	green/yellow
N	Not used	–	–	–
O	Not used	–	–	–
P	Not used	–	–	–
Q	Not used	–	–	–

* Grey wire not used.

** Install jumper between F and G for ORP sensors and pH electrodes without SG.

*** Blue wire for electrode with SG.

4.3.4 TB2 – Oxygen Analog Sensors

		InPro6800(G)	InPro6900	InPro6950
Terminal	Function	Color	Color	Color
A	Not used	–	–	–
B	Anode	red	red	red
C	Anode	–*	–*	–
D	Reference	–*	–*	blue
E	Not used	–	–	–
F	Not used	–	–	–
G	Guard	–	grey	grey
H	Cathode	transparent	transparent	transparent
I	NTC ref (GND)	white	white	white
J	Not used	–	–	–
K	NTC	green	green	green
L	Not used	–	–	–
M	Shield (GND)	green/yellow	green/yellow	green/yellow
N	Not used	–	–	–
O	Not used	–	–	–
P	+ input 4/20 mA signal	–	–	–
Q	– input 4/20 mA signal	–	–	–

* Install jumper between C and D for InPro 6800(G) and InPro 6900

4.3.5 TB2 – pH, Amp. Oxygen, Ozone, Conductivity 4-e and Dissolved CO₂ (Low) ISM (Digital) Sensors

	pH, Amp. Oxygen, Ozone, Cond 4-e, Dissolved CO ₂	
Terminal	Function	Color
A	Not used	–
B	Not used	–
C	Not used	–
D	Not used	–
E	Not used	–
F	Not used	–
G	Not used	–
H	Not used	–
I	Not used	–
J	Not used	–
K	Not used	–
L	1-wire	transparent (cable core)
M	GND	red (shield)
N	RS485-B	–
O	RS485-A	–
P	Not used	–
Q	Not used	–

4.3.6 TB2 – Optical Oxygen, CO₂ hi ISM (Digital) Sensors


Terminal	Optical Oxygen with VP8 Cable*		Optical Oxygen with other Cables**, CO ₂ hi (InPro 5500i)	
	Function	Color	Function	Color
A	Not used	–	Not used	–
B	Not used	–	Not used	–
C	Not used	–	Not used	–
D	Not used	–	Not used	–
E	Not used	–	Not used	–
F	Not used	–	Not used	–
G	Not used	–	Not used	–
H	Not used	–	Not used	–
I	Not used	–	Not used	yellow
J	Not used	–	Not used	–
K	Not used	–	Not used	–
L	Not used	–	Not used	–
M	D_GND (shield)	green/yellow	D_GND (shield)	grey
N	RS485-B	brown	RS485-B	blue
O	RS485-A	pink	RS485-A	white
P	Not used	–	Not used	–
Q	Not used	–	Not used	–


* Connect the grey +24 DC wire and the blue D_GND 24 V wire of the sensor separately.

** Connect the brown +24 DC wire and the black D_GND 24 V wire of the sensor separately.

4.4 Connection of ISM (Digital) Sensors

4.4.1 Connection of ISM Sensors for pH/ORP, Cond 4-e, Amp. Oxygen Measurement and Dissolved CO₂ (Low)

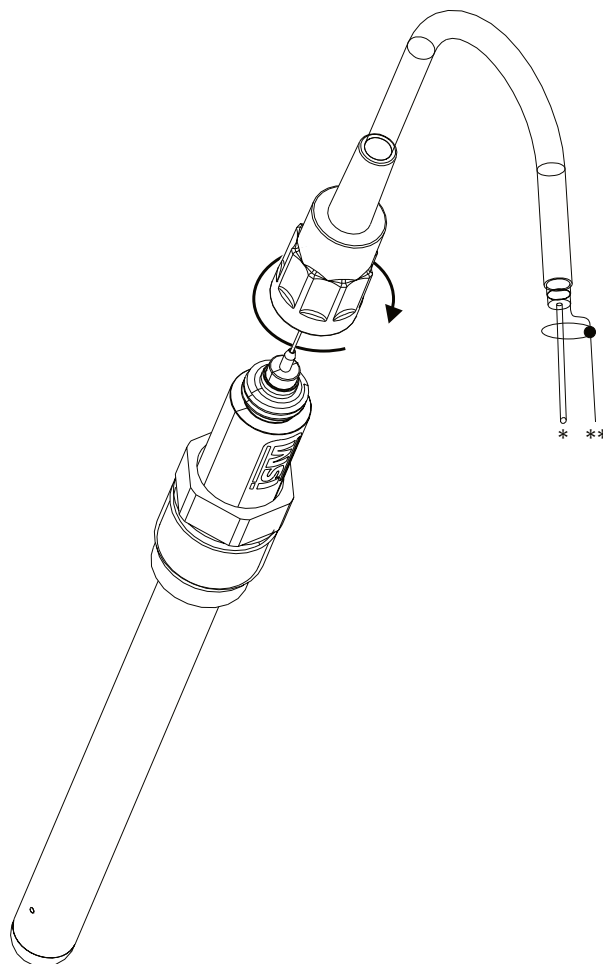


 **NOTE:** Connect the sensor and screw the plug head clockwise (hand tight).


4.4.2 TB2 – AK9 Cable Assignment


* 1-wire data (transparent)

** Ground/shield

4.4.3 Connection of ISM Sensors for Optical Oxygen Measurement and CO₂ hi (InPro 5500i)

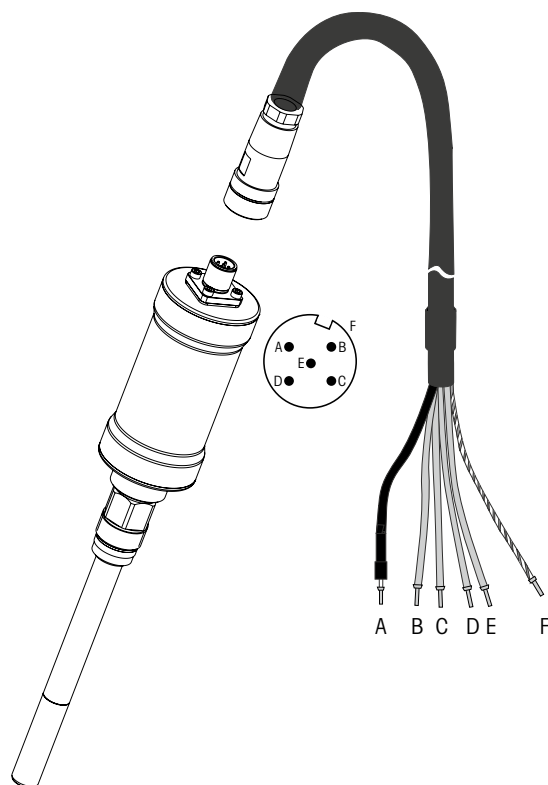


 **NOTE:** Connect the Sensor and screw the plug head clockwise (hand tight).

 **NOTE:** The illustration does not apply for optical oxygen ISM sensors with VP8 cable.

4.5 Connection of Analog Sensors

4.5.1 Connection of Analog Sensor for pH/ORP

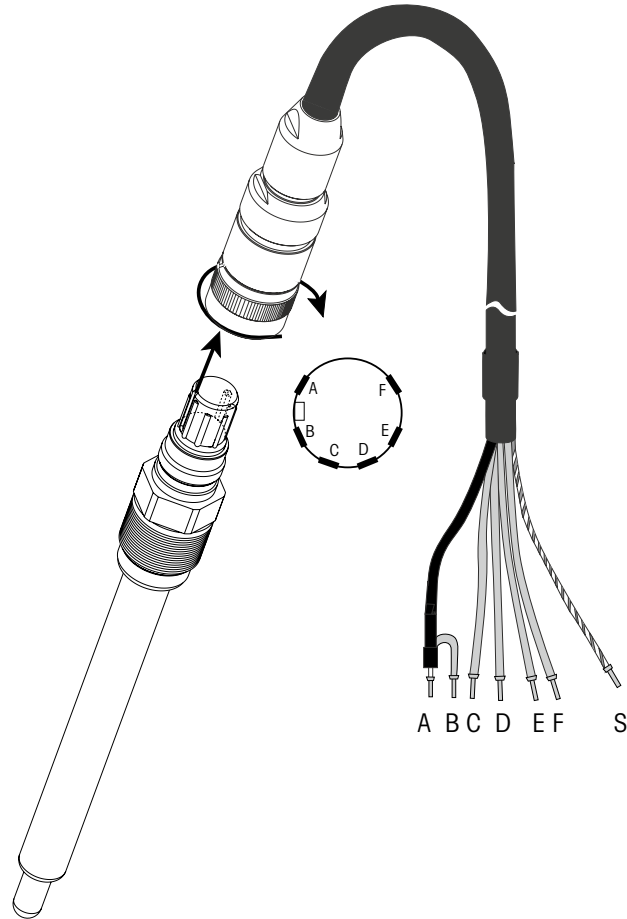


NOTE: Cable lengths > 20 m can worsen the response during pH measurement. Be sure to observe the sensor instruction manual.

4.5.2 TB2 – Typical Wiring for Analog pH/ORP Sensor

4.5.2.1 Example 1

pH measurement without Solution Ground

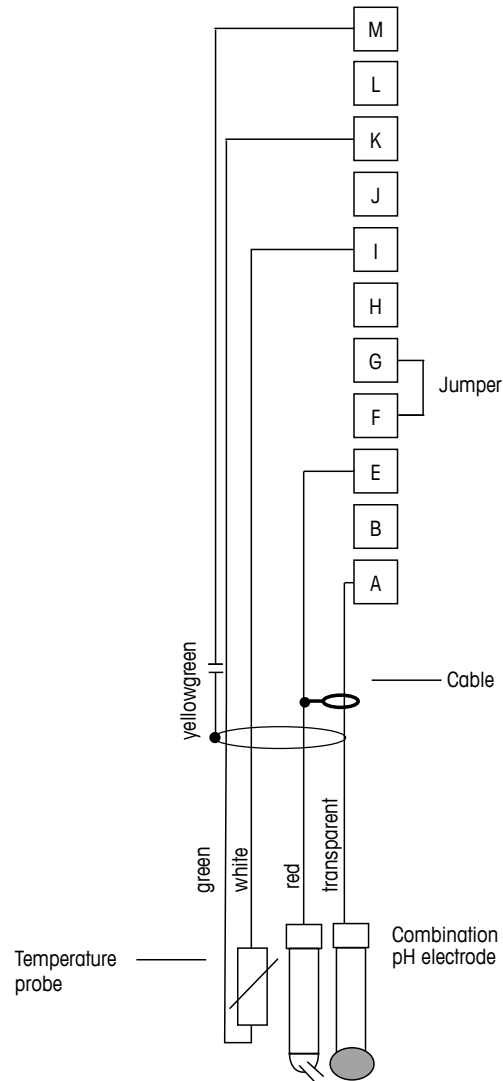

 **NOTE:** Jumper terminals G and F

Wire Colors only valid for connection with VP cable; blue and grey not connected.

A: Glass

E: Reference


I: RTD ret/GND

K: RTD

M: Shield/GND

4.5.2.2 Example 2

pH measurement with Solution Ground

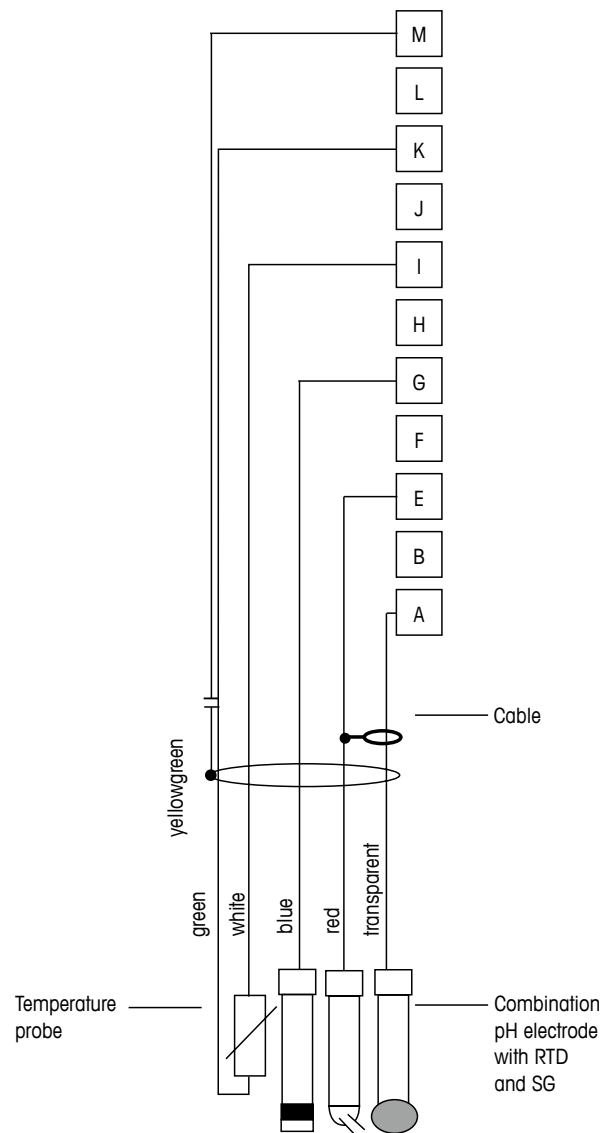


NOTE: Wire colors only valid for connection with VP cable, grey not connected.

- A: Glass
- E: Reference
- G: Shield/Solution GND
- I: GND/RTD ret
- K: RTD
- M: Shield (GND)

4.5.2.3 Example 3

ORP (redox) measurement (temperature optional)

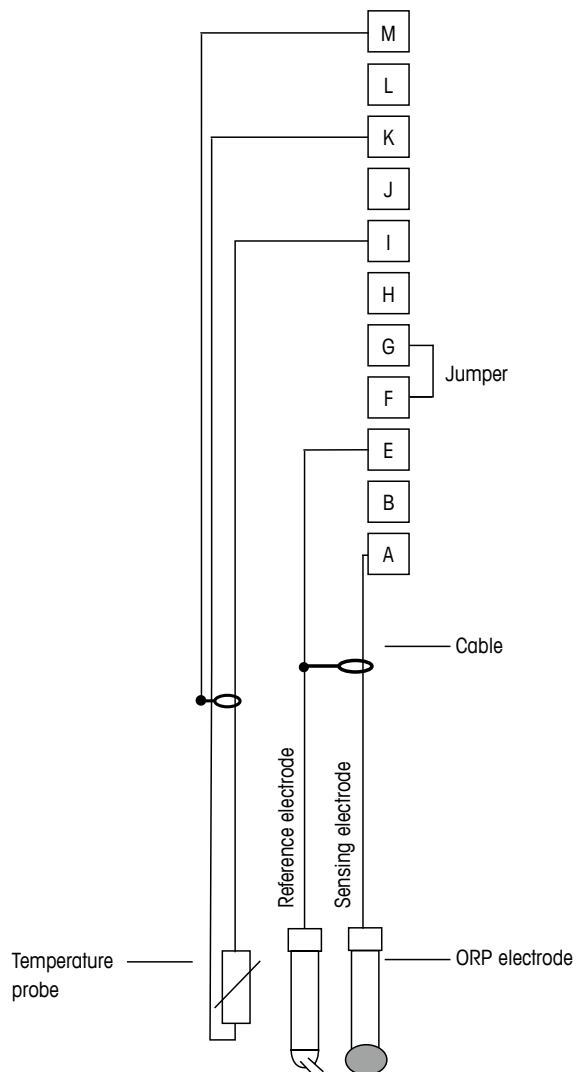


 **NOTE:** Jumper terminal G and F

A: Platinum
 E: Reference
 I: RTD ret/GND
 K: RTD
 M: Shield (GND)

4.5.2.4 Example 4


ORP measurement with pH solution ground electrode (e.g. InPro 3250, InPro 4800SG).

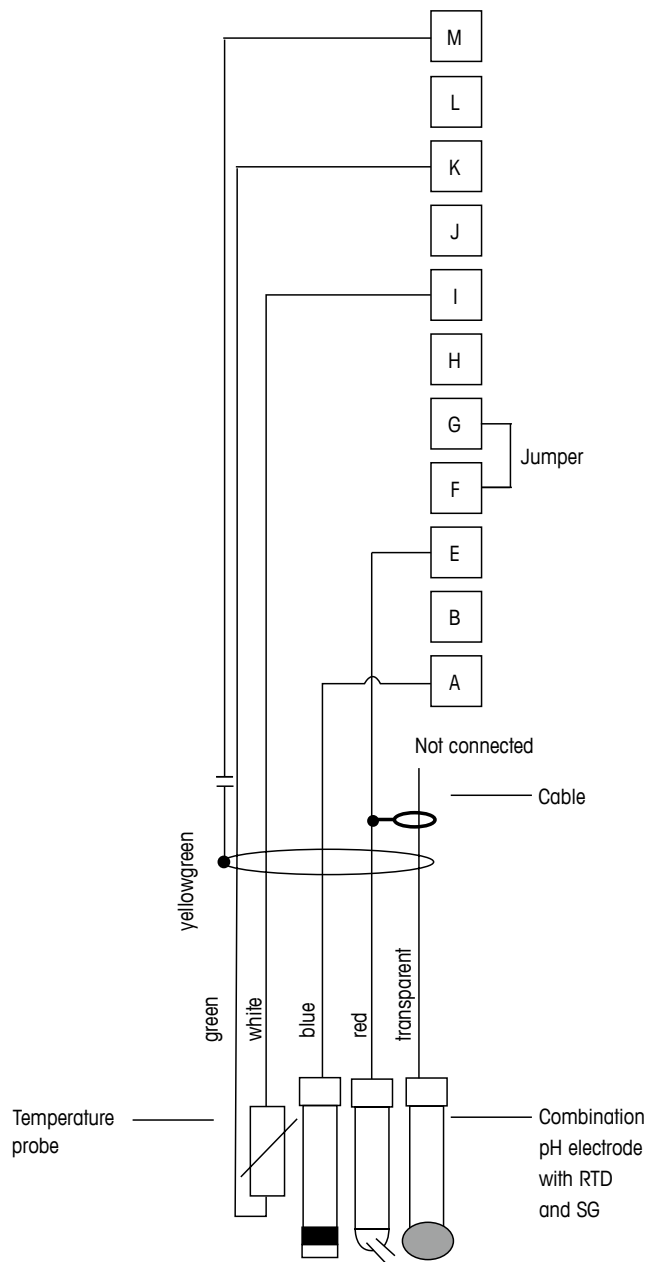

 **NOTE:** Jumper terminal G and F


- A: Platinum
- E: Reference
- I: RTD ret/GND
- K: RTD
- M: Shield (GND)


4.5.3 Connection of Analog Sensor for Amperometric Oxygen Measurement

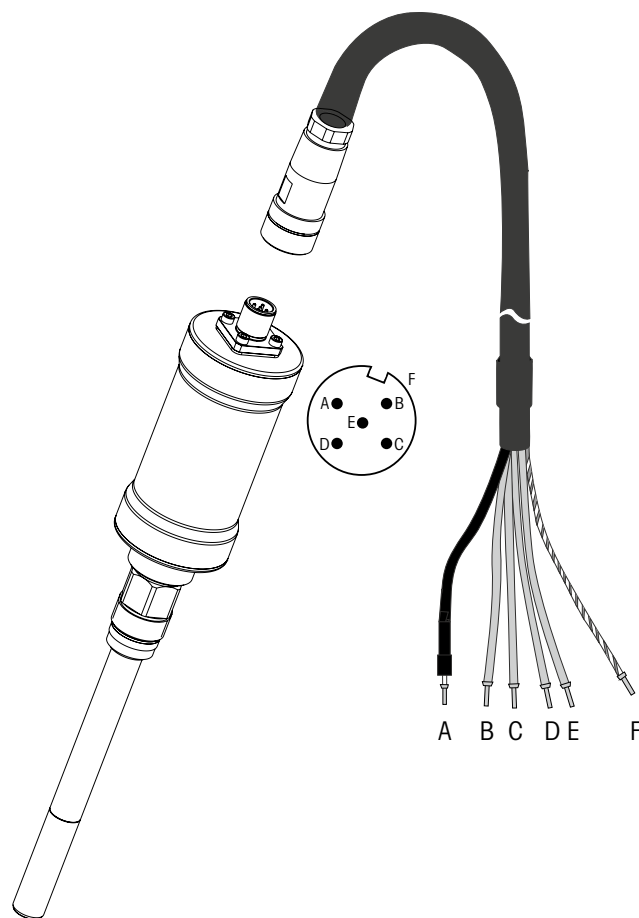

NOTE: Be sure to observe the sensor instruction manual.

4.5.4 TB2 – Typical Wiring for Analog Sensor for Amperometric Oxygen Measurement

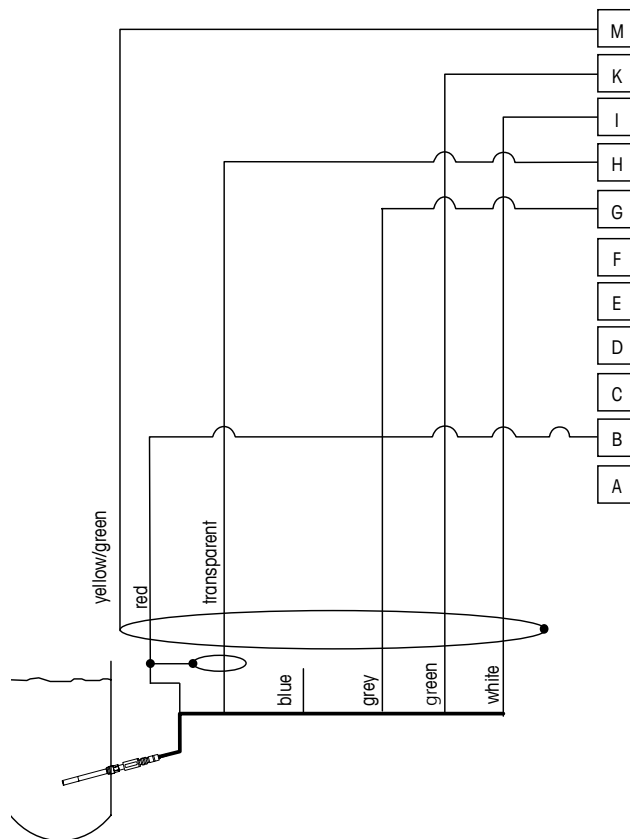

 **NOTE:** Wire colors only valid for connection with VP cable, but not connected.

M400 connector:

- B: Anode
- G: Reference
- H: Cathode
- I: NTC ret/Guard
- K: NTC
- M: Shield (GND)

5 Placing Transmitter In, or Out, of Service

5.1 Placing Transmitter in Service



WARNING: After connecting the transmitter to power supply circuit, it will be active as soon as the circuit is powered.

5.2 Placing Transmitter Out of Service

Switch on power supply. Disconnect the unit from the main power source. Disconnect all remaining electrical connections. Remove the unit from the wall/panel. Use the installation instruction in this manual as reference for dis-assembling mounting hardware.

All transmitter settings stored in memory are non volatile.

6 Quick Setup

(PATH: Menu/Quick Setup)

Select Quick Setup and press the [ENTER] key. Enter the security code if necessary (see section 9.2 "Passwords")



NOTE: Please find the complete description of the Quick Setup routine described in the separate booklet "Quick Setup Guide for Transmitter M400" enclosed in the box.



NOTE: Please do not use Quick Setup menu after configuration of the transmitter, because some of the parameters will may be reseted.



NOTE: Refer to section 3.2 "Control/Navigation Keys" for information on menu navigation.

7 Sensor Calibration


(PATH: Cal)

The calibration key ► allows the user one-touch access to sensor calibration and verification features.



NOTE: During Calibration on Channel A or B, a flashing "H" (Hold) on the left side of the Display indicates a calibration is in process with a Hold condition active. The hold output needs to be activated. See also section 3.2.8 "Display".

7.1 Enter Calibration Mode



While in Measurement mode press the ► key. If the display prompts you to enter the Calibration security code, press the ▲ or ▼ key to set the calibration security mode, the [ENTER] key to confirm the calibration security code.

Press the ▲ or ▼ key to select the type of calibration desired.

7.1.1 Select the Desired Sensor Calibration Task

For analog sensors depending on sensor type, the following choices are available:

Conductivity	= Conductivity, Resistivity, Temperature, Edit, Verify
Amp. Oxygen	= Oxygen, Temperature, Edit, Verify
pH	= pH, ORP, mV, Temperature, Edit pH, Edit mV, Verify

For ISM (digital) sensors depending on sensor type, the following choices are available:

Conductivity	= Conductivity, Resistivity, Verify
Amp. Oxygen	= Oxygen, Verify
Optical Oxygen	= Oxygen, Verify
pH	= pH, ORP, Verify
CO ₂	= CO ₂
Ozone	= O ₃

7.1.2 Finish Calibration

After every successful calibration the following options are available.

After selection the message "RE-INSTALL SENSOR and Press [ENTER]" appears on the display. Press [ENTER] to return to the measuring mode.

Analog sensors

Adjust: Calibration values are stored in the transmitter and used for the measurement. Additionally, the calibration values are stored in the calibration data.

Calibrate: The function "Calibrate" is not applicable for analog sensors.

Abort: Calibration values are discarded.

ISM (digital) sensors

Adjust: Calibration values are stored in the sensor and used for the measurement. Additionally, the calibration values are stored in the calibration history.

Calibrate: Calibration values are stored in the calibration history for documentation, but not be used for the measurement. The calibration values from the last valid adjustment are further used for the measurement.

Abort: Calibration values are discarded.

7.2 Conductivity Calibration for Two- or Four-Electrode Sensors


This feature provides the ability to perform a one-point, two-point or process Conductivity resp. Resistivity "Sensor" calibration for two- or four-electrode sensors. The procedure described below works for both types of calibrations. There is no reason to perform a two-point calibration on a two-electrode conductivity sensor.



NOTE: When performing calibration on a conductivity sensor, results will vary depending on the methods, calibration apparatus and/or quality of reference standards used to perform the calibration.



NOTE: For measuring tasks the temperature compensation for the application as defined at the menu Resistivity will be considered and not the temperature compensation selected thru the calibration procedure (see also section 8.2.3.1 "Conductivity Temperature Compensation"; PATH: Menu/Configure/Measurement/Resistivity).



Enter Conductivity sensor calibration mode as described in section 7.1 "Enter Calibration Mode".

The next screen will ask to select the type of temperature compensation mode desired during the calibration process.



Choices are "None", "Standard", "Light 84", "Std 75 °C", "Lin 25 °C", "Lin 20 °C", "Glycol.5", "Glycol1", "Cation", "Alcohol" and "Ammonia".

None does not make any compensation of the measured conductivity value. The uncompensated value will be displayed and proceeded.

Standard compensation includes compensation for non-linear high purity effects as well as conventional neutral salt impurities and conforms to ASTM standards D1125 and D5391.

Light 84 compensation matches the high purity water research results of Dr. T.S. Light published in 1984. Use only if your institution has standardized on that work.

Std 75 °C compensation is the Standard compensation algorithm referenced to 75 °C. This compensation may be preferred when measuring Ultrapure Water at an elevated temperature (Resistivity of ultrapure water compensated to 75 °C is 2.4818 Mohm-cm.)

Linear 25 °C compensation adjusts the reading by a coefficient or factor expressed as %/°C (deviation from 25 °C). Use only if the solution has a well-characterized linear temperature coefficient. The factory default setting is 2.0% /°C.

Linear 20 °C compensation adjusts the reading by a coefficient or factor expressed as %/°C (deviation from 20 °C). Use only if the solution has a well-characterized linear temperature coefficient. The factory default setting is 2.0% /°C.

Glycol.5 compensation matches the temperature characteristics of 50% ethylene glycol in water. Compensated measurements using this solution may go above 18 Mohm-cm.

Glycol1 compensation matches the temperature characteristics of 100% ethylene glycol. Compensated measurements may go well above 18 Mohm-cm.

Cation compensation is used in power industry applications measuring the sample after a cation exchanger. It takes into account the effects of temperature on the dissociation of pure water in the presence of acids.

Alcohol compensation provides for the temperature characteristics of a 75% solution of isopropyl alcohol in pure water. Compensated measurements using this solution may go above 18 Mohm-cm.


Ammonia compensation is used in power industry applications for specific conductivity measured on samples using ammonia and/or ETA (ethanolamine) water treatment. It takes into account the effects of temperature on the dissociation of pure water in the presence of these bases.

Choose the compensation mode, modify the factor where appropriate and press [ENTER].

7.2.1 One-Point Sensor Calibration


(Display reflects typical Conductivity Sensor calibration)

Enter Conductivity Sensor Calibration mode as described in section 7.1 "Enter Calibration Mode" and choose one of the compensation modes (see section 7.2 "Conductivity Calibration for Two- or Four-Electrode Sensors").




Select 1 point calibration and press [ENTER]. With conductivity sensors a one-point calibration is always performed as a slope calibration.

Place the electrode into the reference solution.



Enter the value for Point 1 including a decimal point and units. The value in the second text line is the value being measured by the transmitter and sensor in the units selected by the user. Press [ENTER] when this value is stable to perform the calibration.




After the calibration the cell multiplier or slope calibration factor "M" i.e. cell constant and the Adder or offset calibration factor "A" are displayed.

For ISM (digital) sensors select ADJUST, CALIBRATE or ABORT to finish calibration. For Analog sensors select ADJUST or ABORT to finish calibration. See "7.1.2 Finish Calibration".

7.2.2 Two-Point Sensor Calibration (Only for Four-Electrode Sensors)

(Display reflects typical Conductivity sensor calibration)


Enter Conductivity Sensor Calibration mode as described in section 7.1 "Enter Calibration Mode" and choose one of the compensation modes (see section 7.2 "Conductivity Calibration for Two- or Four-Electrode Sensors").



Select 2 point calibration and press [ENTER].

Place the electrode into the first reference solution.

CAUTION: Rinse sensors with a high-purity water solution between calibration points to prevent contamination of the reference solutions.



Enter the value for Point 1 including a decimal point and units. The value in the second text line is the value being measured by the transmitter and sensor in the units selected by the user. Press [ENTER] when this value is stable and place the electrode into the second reference solution.

Enter the value for Point 2 including a decimal point and units. The value in the second text line is the value being measured by the transmitter and sensor in the units selected by the user. Press [ENTER] when this value is stable to perform the calibration.




After the calibration of the cell multiplier or slope calibration factor "M" i.e. cell constant and the adder or offset calibration factor "A" are displayed.

For ISM (digital) sensors select ADJUST, CALIBRATE or ABORT to finish calibration. For Analog sensors select ADJUST or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.2.3 Process Calibration

(Display reflects typical Conductivity sensor calibration)

Enter Conductivity Sensor Calibration mode as described in section 7.1 "Enter Calibration Mode" and choose one of the compensation modes (see section 7.2 "Conductivity Calibration for Two- or Four-Electrode Sensors").




Select Process Calibration and press [ENTER]. With conductivity sensors a process calibration is always performed as a slope calibration.




Take a sample and press the [ENTER] key again to store the current measuring value.

During the ongoing calibration process, the letter of the channel, which is concerned by the calibration, "A" or "B" is blinking in the display.

After determining the conductivity value of the sample, press the [CAL] key again to proceed with the calibration.



Enter the conductivity value of the sample, then press the [ENTER] key to start the calculation of calibration results.



After the calibration the Multiplier or slope calibration factor "M" and the Adder or offset calibration factor "A" are displayed.

For ISM (digital) sensors select ADJUST, CALIBRATE or ABORT to finish calibration. For Analog sensors select ADJUST or ABORT to finish calibration. See „7.1.2 Finish Calibration“.


7.3 Calibration of Amperometric Oxygen Sensors

Oxygen calibration for amperometric sensors is performed as either a one-point or process calibration.




NOTE: Before air calibration, for highest accuracy, enter the barometric pressure and relative humidity, as described in section 8.2.3.4 "Parameters for Oxygen Measurement Based on Amperometric Sensors".

7.3.1 One-Point Calibration for Amperometric Oxygen Sensors




Enter Oxygen calibration mode as described in section 7.1 "Enter Calibration Mode".


A one-point calibration of oxygen sensors is always either a one-point slope (i.e. with air) or a zero (offset) calibration. A one-point slope calibration is done in air and a one-point offset calibration is done at 0 ppb oxygen. A one-point zero dissolved oxygen calibration is available but not normally recommended since zero oxygen is very hard to achieve. A zero-point calibration is only recommended if high accuracy at low oxygen level (below 5% air) is needed.



Select 1 point followed by either Slope or ZeroPt as the calibration type. Press [ENTER].



Adjust calibration pressure (CalPres) and relative humidity (RelativeHumid), which are applied during calibration. Press [ENTER].



Place the sensor in the calibration gas (e.g. air) resp. solution. Press [ENTER].

Depending on the parameterized Drift control (see section 8.2.3.4 "Parameters for Oxygen Measurement Based on Amperometric Sensors") one of the two following modes is active.

7.3.1.1 Auto Mode



NOTE: For a zero point calibration the Auto mode is not available. If Auto mode has been configured (see section 8.2.3.4 "Parameters for Oxygen Measurement Based on Amperometric Sensors") and an offset calibration will be executed, the transmitter will perform the calibration in Manual mode.

```

B  98.6  %air
H  25.0  °C

A Point1=100.5 %air  · ↑
A  02=107.4 %air

```

Enter the value for Point 1 including a decimal point and units. The value in the second text line is the value being measured by the transmitter and sensor in the units selected by the user.

```

B  98.6  %air
B  25.0  °C

02 S=-77.02rA Z=0.0000rA
Save Adjust. ↑

```

As soon as the stabilization criteria have been fulfilled the display changes. The display shows the calibration result for slope "S" and offset value "Z".

For ISM (digital) sensors select ADJUST, CALIBRATE or ABORT to finish calibration. For Analog sensors select ADJUST or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.3.1.2 Manual Mode

```

B  98.6  %air
H  25.0  °C

A Point1=100.5 %air  · ↑
A  02=107.4 %air

```

Enter the value for Point 1 including a decimal point and units. The value in the second text line is the value being measured by the transmitter and sensor in the units selected by the user. Press [ENTER] when this value is stable to perform the calibration.

```

B  98.6  %air
B  25.0  °C

02 S=-77.02rA Z=0.0000rA
Save Adjust. ↑

```


After the calibration the slope "S" and the offset value "Z" are displayed.

For ISM (digital) sensors select ADJUST, CALIBRATE or ABORT to finish calibration. For Analog sensors select ADJUST or ABORT to finish calibration. See „7.1.2 Finish Calibration“.



NOTE: With ISM sensors: If a one-point calibration is executed, the transmitter sends the polarization voltage, valid for the calibration, to the sensor. If the polarization voltage for the measuring mode and calibration mode is different, the transmitter will wait 120 seconds before starting the calibration. In this case the transmitter will also go after the calibration for 120 seconds to the HOLD Mode, before returning to the measuring mode again. (see also section 8.2.3.4 "Parameters for Oxygen Measurement Based on Amperometric Sensors").

7.3.2 Process Calibration for Amperometric Oxygen Sensors



Enter Oxygen calibration mode as described in section 7.1 "Enter Calibration Mode".

A process calibration of oxygen sensors is always either a slope or a offset calibration.



Select Process followed by either Slope or ZeroPt as the calibration type. Press [ENTER]




Take a sample and press the [ENTER] key again to store the current measuring value. To show the ongoing calibration process, A or B (depending on the channel) is blinking in the display.

After determining the O₂ value of the sample press the ► key again to proceed with the calibration.



Enter the O₂ value of the sample then press the [ENTER] key to start the calculation of the calibration results.



After the calibration the slope "S" and the offset value "Z" are displayed.

For ISM (digital) sensors select ADJUST, CALIBRATE or ABORT to finish calibration. For Analog sensors select ADJUST or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.4 Calibration of Optical Oxygen Sensors (Only for ISM Sensors)

Oxygen calibration for optical sensors can be performed as a two-point, process or, depending on the sensor model connected to the transmitter, also as a one-point calibration.

7.4.1 One-Point Calibration for Optical Oxygen Sensors

Typically a one-point calibration is done in air. Nevertheless other calibration gases and solutions are possible.

The calibration of an optical sensor is always a calibration of the phase of the fluorescence signal towards the internal reference. During a one-point calibration the phase in this point is measured and extrapolated over the measuring range.

Enter O₂ opt calibration mode as described in section 7.1 "Enter Calibration Mode".

```
B 99.3 %AIR
B 25.0 °C
Calibrate Sensor
Channel B O2 Opt ↑
```

Select 1 point as the calibration type. Press [ENTER].

```
B 99.3 %AIR
H 25.0 °C
O2 Optical Calibration
Type = 1 point ↑
```

Place the sensor in the calibration gas (e.g. air) resp. solution.

```
B 99.3 %air
25.0 °C
CalPres = 759.8 mHq
RelativeHumid = 100 % ↑
```

Adjust calibration pressure (CalPres) and relative humidity (RelativeHumid), which are applied during calibration. Press [ENTER].

```
B 99.3 %air
25.0 °C
Press ENTER when
Sensor is in Gas 1(Air) ↑
```

Place the sensor in the calibration gas (e.g. air) resp. solution. Press [ENTER].

Depending on the parameterized Drift control (see section 8.2.3.5 "Parameters for Oxygen Measurement Based on Optical Sensors") one of the two following modes is active.

7.4.1.1 Auto Mode

```
B 99.3 %AIR
25.0 °C
B Point1=100.0 %AIR ..↑
B 02=99.90 %AIR ↑
```


Enter the value for Point 1 including a decimal point and units. The value in the second text line is the value being measured by the transmitter resp. sensor in the units selected by the user.

```
B 99.3 %AIR
B 25.0 °C
O2 P100=0.00 P0=99.00
Save Adjust ↑
```

As soon as the stabilization criteria have been fulfilled the display changes. The display shows now the values for the phase of the sensor at 100% air (P100) and at 0% (P0) air.


Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.4.1.2 Manual Mode



Enter the value for Point 1 including a decimal point and units. The value in the second text line is the value being measured by the transmitter resp. sensor in the units selected by the user.

Press [ENTER] to proceed.




The display shows now the values for the phase of the sensor at 100% air (P100) and at 0% (P0) air.

Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.


7.4.2 Two-Point Sensor Calibration

The calibration of an optical sensor is always a calibration of the phase of the fluorescence signal towards the internal reference. A two-point calibration is a combination of first a calibration in air (100%) where a new phase P100 is measured and then a calibration in nitrogen (0%) where a new phase P0 is measured. This calibration routine gives the most accurate calibration curve over the whole measuring range.


Enter O₂ opt calibration mode as described in section 7.1 “Enter Calibration Mode“.




Select 2 point as the calibration type. Press [ENTER].



Adjust calibration pressure (CalPres) and relative humidity (RelativeHumid), which are applied during calibration. Press [ENTER].




Place the sensor in the first calibration gas (e.g. air) resp. solution. Press [ENTER].




Depending on the parameterized Drift control (see section 8.2.3.5 “Parameters for Oxygen Measurement Based on Optical Sensors”) one of the two following modes is active.

7.4.2.1 Auto Mode




Enter the value for Point 1 including a decimal point and units. The value in the second text line is the value being measured by the transmitter resp. sensor in the units selected by the user.




As soon as the stabilisation criteria have been fulfilled, the display changes and prompts you to change the gas.

Place the sensor in the second calibration gas and press the [ENTER] key to go on with the calibration.



Enter the value for Point 2 including a decimal point and units. The value in the second text line is the value being measured by the transmitter resp. sensor.



As soon as the stabilization criteria have been fulfilled the display changes. The display shows now the values for the phase of the sensor at 100% air (P100) and at 0% (P0) air.


Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.4.2.2 Manual Mode



Enter the value for Point 1 including a decimal point and units. The value in the second text line is the value being measured by the transmitter resp. sensor in the units selected by the user.

Press [ENTER] to proceed.




The display changes and prompts you to change the gas.

Place the sensor in the second calibration gas and press the [ENTER] key to go on with the calibration.



Enter the value for Point 2 including a decimal point and units. The value in the second text line is the value being measured by the transmitter resp. sensor.

Press [ENTER] to proceed.




The display shows now the values for the phase of the sensor at 100% air (P100) and at 0% (P0) air.

Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.


7.4.3 Process Calibration

The calibration of an optical sensor is always a calibration of the phase of the fluorescence signal towards the internal reference. During a process calibration the phase in this point is measured and extrapolated over the measuring range.

Enter O₂ opt calibration mode as described in section 7.1 "Enter Calibration Mode".



Select 1 point as the calibration type. Press [ENTER].




Take a sample and press the [ENTER] key again to store the current measuring value. To show the ongoing calibration process, A or B (depending on the channel) is blinking in the display.



After determining the O₂ value of the sample press the [CAL] key again to proceed with the calibration.

Enter the O₂ value of the sample then press the [ENTER] key to start calibration.



The display shows now the values for the phase of the sensor at 100% air (P100) and at 0% (P0) air.

Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.




7.5 pH Calibration

For pH sensors, the M400 transmitter features one-point, two-point (Auto or Manual mode) or process calibration with 9 preset buffer sets or manual buffer entry. Buffer values refer to 25 °C. To calibrate the instrument with automatic buffer recognition, you need a standard pH buffer solution that matches one of these values. (See section 8.2.3.3 "pH/ORP Parameters" for configuring modes and selecting buffer sets.) Please select the correct buffer table before using automatic calibration (see section 19 "Buffer Tables").




NOTE: For dual membrane pH electrodes (pH/pNa) only buffer Na+ 3.9M (see section 19.2.1 "Mettler-pH/pNa Buffers (Na+ 3.9M)") is available.

7.5.1 One-Point Calibration




Enter pH calibration mode as described in section 7.1 "Enter Calibration Mode".




Select 1 point Calibration. With pH sensors a one-point calibration is always performed as a offset calibration.

Depending on the parameterized Drift control (see section 8.2.3.3 "pH/ORP Parameters") one of the two following modes is active.


7.5.1.1 Auto Mode



Place the electrode in the buffer solution and press the [ENTER] key to start the calibration.




The display shows the buffer the transmitter has recognized (Point 1) and the measured value.



As soon as the stabilisation criteria have been fulfilled the display changes. The display shows now the slope calibration factor S and the offset calibration factor Z.

For ISM (digital) sensors select ADJUST, CALIBRATE or ABORT to finish calibration. For Analog sensors select ADJUST or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.5.1.2 Manual Mode



Place the electrode in the buffer solution. The display shows the buffer the transmitter has recognized (Point 1) and the measured value. Press [ENTER] to proceed.




The display shows now the slope calibration factor S and the offset calibration factor Z.

For ISM (digital) sensors select ADJUST, CALIBRATE or ABORT to finish calibration. For Analog sensors select ADJUST or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.5.2 Two-Point Calibration




Enter pH calibration mode as described in section 7.1 “Enter Calibration Mode“.




Select 2 Point calibration.

Depending on the parameterized Drift control (see section 8.2.3.3 “pH/ORP Parameters“) one of the two following modes is active.


7.5.2.1 Auto Mode



Place the electrode in the first buffer solution and then press the [ENTER] key.




The display shows the buffer the transmitter has recognized (Point 1) and the measured value.



As soon as the stabilisation criteria have been fulfilled stabilisation criteria have been fulfilled, the display changes and prompts you to place the electrode in the second buffer.

Place the electrode in the second buffer solution and press the [ENTER] key to go on with the calibration.




The display shows the second buffer the transmitter has recognized (Point 2) and the measured value.



As soon as the stabilisation criteria have been fulfilled the display changes to show the slope calibration factor S and the offset calibration factor Z.

For ISM (digital) sensors select ADJUST, CALIBRATE or ABORT to finish calibration. For Analog sensors select ADJUST or ABORT to finish calibration. See „7.1.2 Finish Calibration“.


7.5.2.2 Manual Mode



Place the electrode in the first buffer solution. The display shows the buffer the transmitter has recognized (Point 1) and the measured value. Press [ENTER] to proceed.



Place the transmitter in the second buffer solution. The display shows the buffer the transmitter has recognized (Point 2) and the measured value. Press [ENTER] to proceed.




The display shows the slope calibration factor S and the offset calibration factor Z.

For ISM (digital) sensors select ADJUST, CALIBRATE or ABORT to finish calibration. For Analog sensors select ADJUST or ABORT to finish calibration. See „7.1.2 Finish Calibration“.


7.5.3 Process Calibration




Enter pH calibration mode as described in section 7.1 “Enter Calibration Mode”.




Select Process calibration. With pH sensors a process calibration is always performed as a offset calibration.



Take a sample and press the [ENTER] key again to store the current measuring Value. To show the ongoing calibration process, A or B (depending on the channel) is blinking in the display.



After determining the pH value of the sample, press the [CAL] key again to proceed with the calibration.



Enter the pH value of the sample then press the [ENTER] key to start the calculation of the calibration results.




After the calibration the slope calibration factor S and the offset calibration factor Z are displayed.

For ISM (digital) sensors select ADJUST, CALIBRATE or ABORT to finish calibration. For Analog sensors select ADJUST or ABORT to finish calibration. See „7.1.2 Finish Calibration“.


7.5.4 mV Calibration (Only for Analog Sensors)



Enter mV calibration mode as described in section 7.1 “Enter Calibration Mode”.



The user can now enter Point 1. The offset calibration factor is calculated by using the value of Point1 instead of the measured value (line 4, mV =) and displayed on the next screen.



Z is the newly calculated offset calibration factor. The slope calibration factor S is always 1 and does not enter the calculation.

Select ADJUST or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.5.5 ORP Calibration (Only for ISM Sensors)


In case that an pH sensor with solution ground based on ISM technology is connected to the M400, the transmitter gives the option to make in addition to the pH calibration an ORP calibration.



NOTE: In case of choosing ORP calibration the parameters defined for pH (see section 8.2.3.3 "pH/ORP Parameters", PATH: Menu/Configure/Measurement/pH) will not be considered.



Enter ORP calibration mode as described in section 7.1 "Enter Calibration Mode".



The user can now enter Point 1. In addition the actual ORP is displayed.

Press [ENTER] to proceed.



The display shows the slope calibration factor S and the offset calibration factor Z.

Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.6 Carbon Dioxide Calibration (Only for ISM Sensors)


For dissolved carbon dioxide (CO₂) sensors, the M400 transmitter features one-point, two-point (Auto or Manual mode) or process calibration. For the one-point or two-point calibration the solution with pH = 7.00 and/or pH = 9.21 of the Mettler – 9 standard buffer can be used (see also section 8.2.3.8 "Dissolved carbon dioxide parameters") or the buffer value can be entered manually.

For thermal conductivity CO₂ (CO₂ Hi), please consult the Sensor Manual (InPro 5500 i).

7.6.1 One-Point Calibration




Enter CO₂ calibration mode as described in section 7.1 "Enter Calibration Mode".




Select 1 point Calibration. With CO₂ sensors a one-point calibration is always performed as a offset calibration.

Depending on the parameterized Drift control (see section 8.2.3.8 "Dissolved Carbon Dioxide Parameters") one of the two following modes is active.


7.6.1.1 Auto Mode



Place the electrode in the buffer solution and press the [ENTER] key to start the calibration.



The display shows the buffer the transmitter has recognized (Point 1) and the measured value.



As soon as the stabilisation criteria have been fulfilled the display changes to show the slope calibration factor S and the offset calibration factor Z.

Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.6.1.2 Manual Mode



Place the electrode in the buffer solution. The display shows the buffer the transmitter has recognized (Point 1) and the measured value. Press [ENTER] to proceed.




The display shows now the slope calibration factor S and the offset calibration factor Z.

Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.6.2 Two-Point Calibration



Enter CO₂ calibration mode as described in section 7.1 “Enter Calibration Mode”.



Select 2 Point calibration.

Depending on the parameterized Drift control (see section 8.2.3.8 “Dissolved carbon dioxide parameters”) one of the two following modes is active.

7.6.2.1 Auto Mode

H **137.5** hPa
A **26.1** °C
Press ENTER when
Sensor is in Buffer 1 ↑

Place the electrode in the first buffer solution and press the [ENTER] key to start the calibration.

154.5 hPa
A **26.1** °C
Point1 = 7.00 pH
CO2 = 7.07 pH ↑

The display shows the buffer the transmitter has recognized (Point 1) and the measured value.

122.4 hPa
A **26.1** °C
Press ENTER when
Sensor is in Buffer 2 ↑

As soon as the stabilisation criteria have been fulfilled, the display changes and prompts you to place the electrode in the second buffer.

Place the electrode in the second buffer solution and press the [ENTER] key to go on with the calibration.

2.8 hPa
A **26.1** °C
Point2 = 9.21 pH
CO2 = 8.80 pH ↑

The display shows the second buffer the transmitter has recognized (Point 2) and the measured value.

2.8 hPa
A **26.1** °C
pH S=74.21 % Z=6.948pH
Save Adjust ↑

As soon as the stabilisation criteria have been fulfilled, the display changes to show the slope calibration factor S and the offset calibration factor Z.

Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.6.2.2 Manual Mode

A **122.4** hPa
A **26.1** °C
Point1 = 7.00 pH
CO2 = 7.17 pH ↑

Place the electrode in the first buffer solution. The display shows the buffer the transmitter has recognized (Point 1) and the measured value. Press [ENTER] to proceed.

A **3.1** hPa
A **26.1** °C
Point2 = 9.21 pH
CO2 = 8.77 pH ↑

Place the electrode in the second buffer solution. The display shows the buffer the transmitter has recognized (Point 2) and the measured value. Press [ENTER] to proceed.

2.8 hPa
A **26.1** °C
pH S=74.21 % Z=6.948pH
Save Adjust ↑


The display shows the slope calibration factor S and the offset calibration factor Z.

Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.


7.6.3 Process Calibration




Enter CO₂ calibration mode as described in section 7.1 "Enter Calibration Mode".



Select Process calibration. With CO₂ sensors a process calibration is always performed as a off-set calibration.



Take a sample and press the [ENTER] key again to store the current measuring value. To show the ongoing calibration process, A or B (depending on the channel) is blinking in the display. After determining the CO₂ value of the sample, press the ► key again to proceed with the calibration.



Enter the CO₂ value of the sample then press the [ENTER] key to start calibration.



The display shows the slope calibration factor S and the offset calibration factor Z.

Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.


7.7 Calibration of Ozone Sensors (Only ISM Sensors)

For ozone sensors, the M400 transmitter features one-point zero point or process calibration.


7.7.1 One-Point ZeroPt Calibration for Ozone Sensors




Enter Ozone calibration mode as described in section 7.1 "Enter Calibration Mode".



Select 1 point ZeroPt as the calibration type. Press [ENTER].



Enter the value for Point 1 including a decimal point. Ozone is the value being measured by the transmitter and sensor in the units set by the user. Press [ENTER] when this value is stable to perform the calibration.




As soon as the stabilization criteria have been fulfilled the display changes. The display shows the calibration result for slope "S" and offset value "Z".

Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.7.2


Process Calibration for Ozone Sensors




Enter Ozone calibration mode as described in section 7.1 "Enter Calibration Mode".

An ozone sensor Process calibration is either a Slope or Zero Pt calibration. The Slope calibration is always obtained from a comparison instrument or colorimetric test kit. The Zero Pt calibration is done in air or in ozone-free water.


Select Process followed by either Slope or ZeroPt as the calibration type. Press [ENTER]




Take a sample and press the [ENTER] key again to store the current measuring value.



After determining the O₃ value of the sample press the ► key again to proceed with the calibration.




Enter the O₃ value of the sample. Press the [ENTER] key to start the calculation of the calibration results.



After the calibration the slope "S" and the offset value "Z" are displayed.


Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.8 Sensor Temperature Calibration (Only for Analog Sensors)



Enter Sensor calibration mode as described in section 7.1 "Enter Calibration Mode" and select Temperature.

7.8.1 One-Point Sensor Temperature Calibration



Select 1 Point calibration. Slope or Offset can be selected with the 1 Point calibration. Select Slope to recalculate the Slope factor M (Multiplier) or Offset to recalculate the offset calibration factor A (Adder).



Note: Due to non-linearity the 1 Point Slope temperature calibration is not implemented for the NTC22K as temperature source.



Enter the value for Point 1 and press [ENTER].




Select ADJUST or ABORT to finish calibration. See „7.1.2 Finish Calibration“.


7.8.2 Two-Point Sensor Temperature Calibration



Note: Due to non-linearity the 2 Point temperature calibration is not implemented for the NTC22K as temperature source.



Select 2 Point as calibration type.



Enter the value for Point 1 and press [ENTER].

```

A  1.25  μS/cm
A  25.00  °C
A Point2 = 50.00 °C
A    T = 50.64 °C  ▲

```

Enter the value for Point 2 and press [ENTER].

```

1.25  μS/cm
A  25.00  °C

Temp No:0.99994 R=6.88889
Save Adjust  ↓

```

Select ADJUST, CALIBRATE or ABORT to finish calibration. See „7.1.2 Finish Calibration“.

7.9

Edit Sensor Calibration Constants (Only for Analog Sensors)

```

A  1.25  μS/cm
A  25.00  °C
Calibrate Sensor
Channel A Edit  ▲

```

Enter Calibration mode as described in section 7.1 “Enter Calibration Mode” and select Edit, Edit pH, Edit mV.

```

A  1.25  μS/cm
A  25.00  °C
Ap M=0.1000 A=0.0000
As M=0.1000 A=0.0000  ▲

```

All calibration constants for the selected sensor channel are displayed. Primary measurement constants (p) are displayed on Line 3. Secondary measurement (temperature) constants (s) for the sensor are displayed on Line 4.

The calibration constants can be changed in this menu.

```

A  1.25  μS/cm
A  25.00  °C
Save Calibration Yes
Press ENTER to Exit  ▲

```

Select “Yes2 to save the new calibration values and the successful calibration is confirmed on the display.



NOTE: Each time a new analog conductivity sensor is connected to the M400 transmitter, it is necessary to enter the unique calibration data (cell constant and offset) located on the sensor label.

7.10

Sensor Verification

```

A  1.25  μS/cm
A  25.00  °C
Calibrate Sensor
Channel A Verify  ▲

```

Enter Calibration mode as described in section 7.1 “Enter Calibration Mode” and select “Verify”.

```

A  1.25  μS/cm
A  25.00  °C
Verify Cal:Channel A
Ch A 1.820 MΩ 1.097 KΩ


```

The measured signal of the primary and the secondary measurement in electrical units are shown. The meter calibration factors are used when calculating these values.

Press [ENTER] to exit from this display.

8 Configuration

(PATH: Menu/Configure)

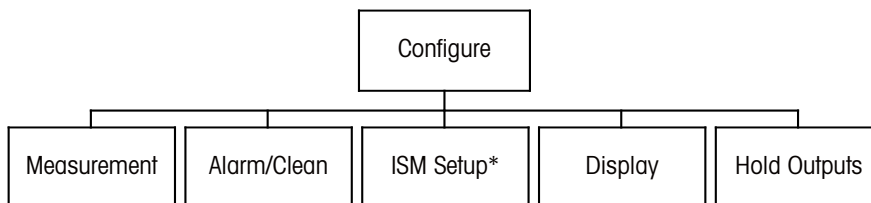

* Only available in combination with ISM sensors


8.1 Enter Configuration Mode



While in Measurement mode, press the ◀ key. Press the ▲ or ▼ key to navigate to the Configure – menu and press [ENTER].

8.2 Measurement

(PATH: Menu/Configure/Measurement)




Enter configuration mode as described in section 8.1 “Enter Configuration Mode”.

Press the [ENTER] key to select this menu. The following sub menus can now be selected: Channel Setup, Temperature Source, Resistivity/Comp/pH/O₂/CO₂, Concentration Table and Set Averaging.

8.2.1 Channel Setup

(PATH: Menu/Configure/Measurement/Channel Setup)



Press the [ENTER] key to select the “Channel Setup” menu.

Depending on the connected sensor (analog or ISM) the channel can be chosen.

8.2.1.1 Analog Sensor



Select sensor type Analog and press [ENTER].

Available measurement types are (depends on transmitter type):

Measurement parameter	Transmitter
pH/ORP = pH or ORP	M400 PA
Cond (2) = 2 electrode conductivity	M400 PA
Cond (4) = 4 electrode conductivity	M400 PA
O ₂ hi = Dissolved oxygen (ppm) or oxygen in gas	M400 PA
O ₂ lo = Dissolved oxygen (ppb) or oxygen in gas	M400 PA
O ₂ Trace = Dissolved oxygen (trace) or oxygen in gas	M400 PA

The 4 lines of the display can now be configured with sensor channel "A" for each line of the display as well as measurements and unit multipliers. Pressing the [ENTER] key will display the selection for lines a, b, c and d.

8.2.1.2 ISM Sensor



Select sensor type ISM and press [ENTER].

If an ISM sensor is connected, the transmitter automatically (Parameter = Auto) recognizes the type of sensor. You can also fix the transmitter to a certain measurement parameter (Parameter = pH/ORP, pH/pNa, Cond(4), O₂ hi, O₂ lo, O₂ Trace, ppm O₂G, O₂ Opt, CO₂ (low)), depending on the type of transmitter you have.


Measurement parameter	Transmitter
pH/ORP = pH and ORP	M400 PA
pH/pNa = pH and ORP (with pH/pNa electrode)	M400 PA
Cond (4) = 4 electrode conductivity	M400 PA
O ₂ hi = Dissolved oxygen (ppm) or oxygen in gas	M400 PA
O ₂ lo = Dissolved oxygen (ppb) or oxygen in gas	M400 PA
O ₂ Trace = Dissolved oxygen (trace) or oxygen in gas	M400 PA
O ₂ Opt = Dissolved oxygen optical	M400 PA
Ozone	M400 PA
CO ₂ hi = Thermal conductivity CO ₂ (InPro 5500i)	M400 PA

The 4 lines of the display can now be configured with sensor channel "B" for each line of the display as well as measurements and unit multipliers. Pressing the [ENTER] key will display the selection for lines a, b, c and d.



NOTE: Beside the measurement values pH, O₂, T, etc. also the ISM values DLI, TTM and ACT can be assigned to the different lines and linked to the Analog Input Block of the PROFIBUS PA interface. For more information see documentation "PROFIBUS PA parameter Multi-parameter Transmitter M400 PA" on the website "<http://www.mt.com/m400-2wire>".

8.2.1.3 Save Changes of the Channel Setup



After the procedure of the channel setup described in the previous section pressing the [ENTER] key again will bring up the Save Changes dialog. Selecting No will discard the entered values and return to the measurement display screen, selecting Yes will save changes made.

8.2.2 Temperature Source (Only for Analog Sensors)

(PATH: Menu/Configure/Measurement/Temperature Source)



Enter Measurement as described in section 8.2 "Measurement". Select Temperature Source by using the ▲ or ▼ key and press [ENTER].




The following options can be chosen:

- Auto: The transmitter automatically recognizes the temperature source.
- Use NTC22K: Input will be taken from the sensor attached.
- Use Pt1000: Temperature input will be taken from the sensor attached.
- Use Pt100: Input will be taken from the sensor attached.
- Fixed = 25 °C: Allows a specific temperature value to be entered. It must be chosen when customer use pH sensor without temperature source.



NOTE: If temperature source is set to Fixed, the temperature applied during one-point and/or two-point calibration of pH electrodes can be adjusted within the corresponding calibration procedure. After the calibration the fixed temperature defined in this configuration menu is valid again.

Pressing the [ENTER] key will bring up the Save Changes dialog.



Selecting No will discard the entered values and return to the measurement display screen, selecting Yes will save changes made.

8.2.3 Parameter Related Settings


(PATH: Menu/Configure/Measurement/pH, O₂, O₂ optical, O₂ opt sampling rate, LED Mode or Resistivity, Concentration Table or CO₂)

Additional measurement and calibration parameters can be set for each parameter; conductivity, pH, O₂ and CO₂.



NOTE: Use pH menu for settings of pH/pNa sensors.

Enter Configuration Mode as described in section 8.1 "Enter Configuration Mode" and select the menu Measurement (see section 8.2 "Measurement").



Depending on the connected sensor, the menu pH, O₂, CO₂ can be selected by using the ▲ or ▼ key. Press [ENTER]

For more details, please see the following explanations depending on the selected parameter.

8.2.3.1 Conductivity Temperature Compensation

If during the channel setup (see section 8.2.1 "Channel Setup") the parameter conductivity has been chosen or an four-electrode conductivity sensor based on ISM technology is connected to the transmitter, the temperature compensation mode can be selected. Temperature compensation should be matched to the characteristics of the application. The transmitter considers this value for the temperature compensation by calculating and displaying the result for the measured conductivity.



NOTE: For calibration purposes the temperature compensation as defined at the menu "Cal/Compensation" for the buffers resp. samples will be considered (see also section 7.2 "Conductivity Calibration for Two- or Four-Electrode Sensors" resp.)

For doing this adjustment the menu "Resistivity", that will be displayed, has to be chosen (see section 8.2.3 "Parameter Related Settings").

The first two measurement lines are displayed on the screen. This section described the procedure for the first measurement line. By using the key ► the second line will be chosen. To select the 3rd and 4th line press [ENTER]. The procedure itself works at every measurement line in the same way.

Choices are "None", "Standard", "Light 84", "Std 75 °C", "Lin 25 °C", "Lin 20 °C", "Glycol.5", "Glycol1", "Cation", "Alcohol" and "Ammonia".



Standard compensation includes compensation for non-linear high purity effects as well as conventional neutral salt impurities and conforms to ASTM standards D1125 and D5391.

None does not make any compensation of the measured conductivity value. The uncompensated value will be displayed and proceeded.

Light 84 compensation matches the high purity water research results of Dr. T.S. Light published in 1984. Use only if your institution has standardized on that work.

Std 75 °C compensation is the Standard compensation algorithm referenced to 75 °C. This compensation may be preferred when measuring Ultrapure Water at an elevated temperature (Resistivity of ultrapure water compensated to 75 °C is 2.4818 Mohm-cm.)

Glycol.5 compensation matches the temperature characteristics of 50% ethylene glycol in water. Compensated measurements using this solution may go above 18 Mohm-cm.

Glycol1 compensation matches the temperature characteristics of 100% ethylene glycol. Compensated measurements may go well above 18 Mohm-cm.

Cation compensation is used in power industry applications measuring the sample after a cation exchanger. It takes into account the effects of temperature on the dissociation of pure water in the presence of acids.

Alcohol compensation provides for the temperature characteristics of a 75% solution of isopropyl alcohol in pure water. Compensated measurements using this solution may go above 18 Mohm-cm.

Ammonia compensation is used in power industry applications for specific conductivity measured on samples using ammonia and/or ETA (ethanolamine) water treatment. It takes into account the effects of temperature on the dissociation of pure water in the presence of these bases.

Linear 25 °C compensation adjusts the reading by a coefficient or factor expressed as %/°C (deviation from 25 °C). Use only if the solution has a well-characterized linear temperature coefficient.

The factory default setting is 2.0% /°C.


Linear 20 °C compensation adjusts the reading by a coefficient or factor expressed as %/°C (deviation from 20 °C). Use only if the solution has a well-characterized linear temperature coefficient.

The factory default setting is 2.0% /°C.

If compensation mode "Lin 25 °C" or "Lin 20 °C" has been chosen, the factor for the adjustment of the reading can be modified after pressing [ENTER] (If working at measurement line 1 or 2 press [ENTER] twice).

Adjust the factor for temperature compensation.

Pressing [ENTER] will bring up the Save Changes dialog. Selecting No will discard the entered values and return to the measurement display screen, selecting Yes will save changes made.



8.2.3.2 Concentration Table

If during the channel setup (see section 8.2.1 "Channel Setup") the parameter conductivity has been chosen or an four-electrode conductivity sensor based on ISM technology is connected to the transmitter, a concentration table can be defined.

To specify customers-specific solutions, up to 5 concentration values can be edited in a matrix together with up to 5 temperatures. To do so the desired values are edited under the concentration table menu. Furthermore the conductivity values for the according temperature and concentration values are edited.

For doing the settings the menu "Concentration Table", that will be displayed, has to be chosen. (see section 8.2.3 "Parameter Related Settings").




Define the desired **unit**.

Press [ENTER]




NOTE: Refer to section 8.2.1 "Channel Setup" to choose the unit used in the display.




Enter the amount of desired temperature points (**Temp Point**) and **Concentration Points**.

Press [ENTER]



Enter the values for the different concentrations (**ConcentrationX**).

Press [ENTER]



Enter the value of the 1st temperature (**Temp1**) and the value for the conductivity which belongs to the first concentration at this temperature.

Press [ENTER]

Enter the value for the conductivity which belongs to the second concentration at the first temperature and press [ENTER] etc..

After entering all conductivity values, that belong to the different concentrations at the first temperature point, enter in the same way the value of the 2nd temperature point (**Temp2**) and the conductivity value which belongs at the second temperature to the first concentration. Press [ENTER] and go on in the same way for the next concentration points as described for the first temperature point.

Enter in this way the values at every temperature point. After entering the last value, pressing [ENTER] again will bring up the Save Changes dialog. Selecting No will discard the entered values and return to the measurement display screen, selecting Yes will save changes made.



NOTE: The values for the temperature have to increase from Temp1 to Temp2 to Temp3 etc.. The values for the concentration have to increase from Concentration1 to Concentration2 to Concentration3 etc.



NOTE: The conductivity values at the different temperatures have to increase or decrease from Concentration1 to Concentration2 to Concentration3 etc.. Maxima and/or minima are not permitted. If the conductivity values at Temp1 are increasing with the different concentrations, they have to increase also at the other temperatures. If the conductivity values at Temp1 are decreasing with the different concentrations, they have to decrease also at the other temperatures.

8.2.3.3 pH/ORP Parameters

If during the channel setup (see section 8.2.1 "Channel Setup") the parameter pH/ORP has been chosen or an pH sensor based on ISM technology is connected to the transmitter, the parameters drift control, buffer recognition, STC, IP, fixed Calibration temperature and the displayed units for slope and zero point can be set resp. adjusted.

For doing this adjustments resp. settings the menu "pH", that will be displayed, has to be chosen. (see section 8.2.3 "Parameter Related Settings").




Select the **drift control** for calibration as Auto (drift and time criteria have to be fulfilled) or manual (The user can decide when a signal is stable enough to complete calibration) followed by the relevant buffer table for the automatic buffer recognition. If the drift rate is less than 0.4 mV over a 19 second interval then the reading is stable and the calibration is done using the last reading. If the drift criteria is not met within 300 seconds then the calibration times out and the message "Calibration Not Done" Press ENTER Enter to "Exit" is displayed.

Press [ENTER]

For automatic **buffer recognition** during calibration, select the buffer solution set that will be used: Mettler-9, Mettler-10, NIST Tech, NIST Std = JIS Std, HACH, CIBA, MERCK, WTW, JIS Z 8802 or None. See section 19 "Buffer tables" for buffer values. If the auto buffer feature will not be used or if the available buffers are different from those above, select None. Press [ENTER].



NOTE: For dual membrane pH electrodes (pH/pNa) only buffer Na+ 3.9M (see section 19.2.1 "Mettler-pH/pNa Buffers (Na+ 3.9M)") is available.




STC is the solution temperature coefficient in units of pH/°C referenced to 25 °C (Default = 0.000 for most applications). For pure waters, a setting of 0.016 pH/°C should be used. For low conductivity power plant samples near 9 pH, a setting of 0.033 pH/°C should be used. These positive coefficients compensate for the negative temperature influence on the pH of these samples. Press [ENTER].



IP is the isothermal point value (Default = 7.000 for most applications). For specific compensation requirements or non standard inner buffer value, this value can be changed. Press [ENTER].



STC RefTemp sets the temperature to which solution temperature compensation is referenced. The displayed value and the output signal is referenced to STC RefTemp. Selecting "No" means solution temperature compensation is not used. The most common reference temperature is 25 °C. Press [ENTER].



The units for the slope and the zero point, that will be shown on the display can be chosen. The default setting for the unit of the slope is [%] and can be changed to [pH/mV]. For the zero point the default setting of the unit is [pH] and can be changed to [mV]. Use the ► key to move to the input field and select the unit by using the ▲ or ▼ key.

Pressing [ENTER] again will bring up the Save Changes dialog. Selecting No will discard the entered values and return to the measurement display screen, selecting Yes will save changes made.

8.2.3.4 Parameters for Oxygen Measurement Based on Amperometric Sensors

If during the channel setup (see section 8.2.1 "Channel Setup") the parameter O₂ hi, O₂ lo or O₂ Trace has been chosen or an oxygen sensor based on ISM technology is connected to the transmitter, the parameters calibration pressure, process pressure, ProcCalPres, salinity and relative humidity can be set resp. adjusted. If an ISM sensor is connected, there is furthermore the option to adjust the parameterization voltage.

For doing this adjustments resp. settings the menu "O₂", that will be displayed, has to be chosen. (see section 8.2.3 "Parameter Related Settings")



Enter the Calibration pressure in line 3. The default value for CalPres is 759.8 and the default unit is mmHg.

Select Edit in line 4 for entering the applied process pressure manually. Select Ain if an analog input signal is used for the applied process pressure. Select PA if the pressure compensation value is supplied via PA. Press [ENTER]



If Edit has been chosen an input field for entering the value manually is displayed. In case that Ain has been selected the start value (4mA) and the end value (20 mA) of the range for the 4 to 20 mA input signal have to be entered.

Press [ENTER]



For the algorithm of the process calibration the applied pressure (ProcCalPres) has to be defined. The value of the process pressure (ProcPres) or the calibration pressure (CalPres) can be used. Chose the pressure, that applies during the process calibration, resp. should be used for the algorithm.


Select the required Drift Control of the measuring signal during the calibration procedure. Choose Manual if the user will decide when a signal is stable enough to complete the calibration. Select Auto and an automatic stability control of the sensor signal during calibration through the transmitter will be done. Press [ENTER]



In the next step the salinity of the measured solution can be modified.

In addition the relative humidity of the calibration gas can also be entered. The allowed values for relative humidity are in the range 0% to 100%. When no humidity measurement is available, use 50% (default value).

Press [ENTER]



If an ISM sensor has been connected resp. configured there is furthermore the option to adjust the polarization voltage for the sensor. Different value can be entered for the measuring mode (Umeaspol) and for the calibration mode (Ucalpol). For entered values 0 mV to -550 mV the connected sensor will be set to a polarization voltage of -500mV. If the entered value is less then -550mV, the connected sensor will set to a polarization voltage of -674mV.




NOTE: During a process calibration, the polarization voltage Umeaspol, defined for the measuring mode, will be used.



NOTE: If a one-point calibration is executed, the transmitter sends the polarization voltage, valid for the calibration, to the sensor. If the polarization voltage for the measuring mode and calibration mode is different, the transmitter will wait 120 seconds before starting the calibration. In this case the transmitter will also go after the calibration for 120 seconds to the HOLD Mode, before returning to the measuring mode again.

Press [ENTER]



The display shows the Save Changes dialog. Selecting No will discard the entered values and return to the measurement display screen, selecting Yes will save changes made.

8.2.3.5 Parameters for Oxygen Measurement Based on Optical Sensors

If during the channel setup (see section 8.2.1 “Channel Setup”) the parameter O₂ Opt has been chosen, the parameters calibration pressure, process pressure, ProCalPres, salinity, drift control and relative humidity can be set resp. adjusted.

For doing these adjustments the menu “O₂ optical”, that will be displayed, has to be chosen. (see section 8.2.3 “Parameter Related Settings”)

Press [ENTER]



Enter the calibration pressure (line 3). The default value for CalPres is 759.8 and the default unit is mmHg.

Select Edit in line 4 for entering the applied process pressure manually. Select Ain if an analog input signal is used for the applied process pressure. Press [ENTER]




If Edit has been chosen an input field for entering the value manually is displayed. In case that Ain has been selected the start value (4 mA) and the end value (20 mA) of the range for the 4 to 20 mA input signal have to be entered.

Press [ENTER]




NOTE: Refer to section 4.3.6 “TB2 – Optical Oxygen, CO₂ hi ISM (Digital) Sensors”.



For the algorithm of the process calibration the applied pressure (ProcCalPres) has to be defined. The value of the process pressure (ProcPres) or the calibration pressure (CalPres) can be used. Chose the pressure, that applies during the process calibration, resp. should be used for the algorithm.

Select the drift control for calibration as Auto (drift and time criteria have to be fulfilled) or manual (The user can decide when a signal is stable enough to complete calibration). If Auto is selected, the drift is checked by the sensor. If the drift criteria is not met within a defined time (depending on the sensor model) the calibration times out and the message “Calibration Not Done” Press ENTER Enter to “Exit” is displayed.

Press [ENTER]



In the next step the salinity of the measured solution can be modified.

In addition the relative humidity of the calibration gas can also be entered. The allowed values for relative humidity are in the range 0% to 100%. When no humidity measurement is available, use 50% (default value).

Press [ENTER]




Select through the parameter **ProcCal** between Scaling and Calibration for process calibration. If Scaling has been chosen, the calibration curve of the sensor will be untouched, but the output signal of the sensor will be scaled. In case of calibration value <1%, the offset of the sensor output signal will be modified during scaling, for value >1% the slope of the sensor output will be adjusted. For further information about scaling refer to the sensor manual.

Pressing the [ENTER] key again will bring up the Save Changes dialog. Selecting No will discard the entered values and return to the measurement display screen, selecting Yes will save changes made.

8.2.3.6 Adjusting Sampling Rate for Optical Sensors

If during the channel setup (see section 8.2.1 "Channel Setup") the parameter O₂ Opt has been chosen the parameter O₂ opt sampling rate can be adjusted.

For doing this adjustment the menu "O₂ opt sampling rate" has to be chosen (see section 8.2.3 "Parameter Related Settings").



The time interval from one measuring cycle of the sensor to the other can be adjusted i.e. adapted to the application. A higher value will increase the life time of the OptoCap of the sensor.

Pressing the [ENTER] key will bring up the Save Changes dialog. Selecting No will discard the entered values and return to the measurement display screen, selecting Yes will save changes made.

8.2.3.7 LED Mode

If during the channel setup (see section 8.2.1 "Channel Setup") the parameter O₂ Opt has been chosen the parameters LED, T off, DI 1 LED control can be set resp. adjusted.

For doing these adjustments the menu "LED Mode" has to be chosen (see section 8.2.3 "Parameter Related Settings").



The operation mode for the LED of the sensor can be selected. There are the following options.

Off: LED is permanently switched off.

On: LED is permanently switched on.

Auto: The LED is switched on as long as the measured media temperature is smaller then Toff (see next value) or switched off thru the digital input signal (see over next value).



NOTE: If the LED is switched off, no oxygen measurement is performed.

Press [ENTER]



Depending on the measured media temperature the LED of the sensor can be automatically switched off. If the media temperature is higher then Toff, the LED will switched off. The LED will be switched on as soon as the media temperature falls below Toff - 3K. This function give the option to increase the lifetime of the OptoCap by switching off the LED thru SIP or CIP cycles.



NOTE: This function is only active if the operation mode of the LED is set to "Auto".

Press [ENTER]



The operation mode of the sensor LED can also be influenced by the digital input signal DI1 of the transmitter. If the parameter "DI 1 LED control" is set to Yes, the LED is switched off, if DI1 is active. If "DI 1 LED control" is set to No, the signal of DI1 has now influence on the operation mode of the sensor LED.

This function is helpful for remote control of the sensor thru a SPS or DCS.




NOTE: This function is only active if the operation mode of the LED is set to "Auto".

Pressing the [ENTER] key will bring up the Save Changes dialog. Selecting No will discard the entered values and return to the measurement display screen, selecting Yes will save changes made.

8.2.3.8 Dissolved Carbon Dioxide Parameters

If during the channel setup (see section 8.2.1 "Channel Setup") the parameter CO₂ has been chosen, the parameters drift control, salinity, HCO₃, TotPres and the displayed units for slope and zero point can be set resp. adjusted.

For doing this adjustment resp. settings the menu "CO₂", that will be displayed, has to be chosen. (see section 8.2.3 "Parameter Related Settings")



Select **Drift Control** for calibration as Auto (drift and time criteria have to be fulfilled) or manual (the user can decide when a signal is stable enough to complete calibration) followed by the relevant buffer table for the automatic buffer recognition. If the drift rate is less than 0.4 mV over a 19 second interval then the reading is stable and the calibration is done using the last reading. If the drift criteria is not met within 300 seconds then the calibration times out and the message "Calibration Not Done Press ENTER to Exit" is displayed.

For automatic **buffer recognition** during calibration, select the buffer Mettler-9. Use for calibration purposes solution with pH = 7.00 and/or pH = 9.21. If the auto buffer feature will not be used or if the available buffers are different from those above, select None. Press [ENTER] to go on.




The **Salinity** describes the total amount of solved salts in the CO₂ electrolyte of the sensor connected to the transmitter. It is a sensor specific parameter. The default value (28.00 g/L) is valid for the InPro 5000. Do not change this parameter if the InPro 5000 will be used.

The parameter **HCO₃** describes the concentration of hydrogen carbonate in the CO₂ electrolyte of the sensor connected to the transmitter. It is also a sensor specific parameter. The default value 0.050 Mol/L is valid for the InPro 5000. Do not change this parameter if the InPro 5000 will be used.

To go on press [ENTER] again.



If the unit for the measured dissolved carbon dioxide is %sat, the pressure during the calibration resp. measurement has to be considered. This will be done by setting the parameter TotPres. If another unit then %sat has been selected, the result will not be influenced by this parameter.




The units for the slope and the zero point, that will be shown on the display can be chosen. The default setting for the unit of the slope is [%] and can be changed to [pH/mV]. For the zero point the default setting of the unit is [pH] and can be changed to [mV]. Use the ► key to move to the input field and select the unit by using the ▲ or ▼ key.


Pressing [ENTER] again will bring up the Save Changes dialog. Selecting No will discard the entered values and return to the measurement display screen, selecting Yes will save changes made.

8.2.3.9 Thermal Conductivity Dissolved Carbon Dioxide Parameters

If during the channel setup (see section 8.2.1 "Channel Setup") the parameter CO₂ Hi has been chosen, the parameters drift control, CO₂ solubility, temperature factor can be set resp. adjusted.



Select **Drift Control** for calibration as auto (calibration is completed automatically based on meeting drift and time criteria) or manual (the user decides when the CO₂ signal is stable enough to complete a calibration).



The sensor is delivered factory calibrated and is set up to measure in beer as the default.

The sensor offers a choice of CO₂ solubility for measurement in beer or water. For other beverages the user has the possibility to enter individual values for CO₂ solubility and temperature factor.

Default values for measurement in beer (Valid for temperatures –5 ... 50 °C):

CO₂ solubility (A): 1.420 g/L

Temp. factor (B): 2485

Values for pure water:

CO₂ solubility (A): 1.471 g/L

Temp. factor (B): 2491

Values for coke:

CO₂ solubility (A): 1.345 g/L

Temp. factor (B): 2370



For beverages where the user knows the exact CO₂ solubility and the temperature factor the values can be changed individually. If the user desires to evaluate the solubility and temperature factors they can be evaluated with the following formulas.

$$HCO_2 = A * \exp(B * (1/T - 1/298.15))$$

$$cCO_2 = HCO_2 * pCO_2$$

HCO₂ : Calculated CO₂ Solubility (Henry constant) at measured process temp.

A: Solubility of CO₂ (g/L at 25 °C)

B: Temperature factor (valid for –5 ... 50 °C)

cCO₂: Calculated CO₂ concentration

8.2.4 Set Averaging

Enter Configuration Mode as described in section 8.1 "Enter Configuration mode" and select the menu Measurement (see section 8.2 "Configuration/Measurement").




Selected the menu "Set Averaging" by using the ▲ or ▼ key. Press [ENTER]

The averaging method (noise filter) for each measurement line can now be selected. The options are Special (Default), None, Low, Medium and High:



- None = no averaging or filtering
- Low = equivalent to a 3 point moving average
- Medium = equivalent to a 6 point moving average
- High = equivalent to a 10 point moving average
- Special = averaging depending on signal change (normally High averaging but Low averaging for large changes in input signal)




Pressing the [ENTER] key again will bring up the Save Changes dialog. Selecting No will discard the entered values and return to the measurement display screen, selecting Yes will save changes made.

8.3 Alarm/Clean

(PATH: Menu/Configure/Alarm/Clean)

Enter configuration mode as described in section 8.1 "Enter Configuration Mode".



8.3.1 Alarm



This menu allows the configuration of alarm functionality for the display. Via PROFIBUS PA interface you can read out the alarm status supplied by the Discrete Input Block. For more information see documentation "PROFIBUS PA parameter Multi-parameter Transmitter M400 PA" on the website "<http://www.mt.com/m400-2wire>".


To select "Setup Alarm", press the ▲ or ▼ key. Confirm selection with [ENTER].



To select "Alarm event", press the ▲ or ▼ key. To navigate to "No/Yes", press the ◀ and ▶ keys. Confirm selection with [ENTER].

One of the following events may be alarmed:

1. Power failure
2. Software failure
3. Rg diagnostics – pH glass membrane resistance (only for pH,; pH/pNa Rg diagnostics detect both pH and pNa membrane glasses)
4. Rr diagnostics – pH reference resistance (only for pH sensors; except pH/pNa)
5. Cond cell open (only for analog cond 2-e/4-e sensors)
6. Cond cell shorted (only for analog cond 2-e/4-e sensors)
7. Channel B disconnected (only for ISM sensors)
8. Shaft error (only for optical sensors)
9. Signal error (only for optical sensors)
10. Hardware error (only for optical sensors)
11. Dry Cond sensor (only for ISM cond sensors)
12. Cell deviation (only for ISM cond sensors)
13. Electrolyte low (only for ISM amperometric oxygen sensors)



If any of these criteria are set to Yes and the conditions for an alarm are given, the flashing symbol \triangle will be shown in the display, an alarm message will be recorded (see also section 11.1 "Messages"; PATH: Info/Messages).

Via PROFIBUS PA interface you can read out the alarm status supplied by the Discrete Input Block. For more information see documentation "PROFIBUS PA parameter Multi-parameter Transmitter M400 PA" on the website "<http://www.mt.com/m400-2wire>".

The conditions for alarms are:

1. There is a power failure or power cycling
2. The software watchdog performs a reset
3. Rg is out of tolerance – for example, broken measuring electrode (only for pH; pH/pNa Rg diagnostics detect both pH and pNa membrane glasses)
4. Rr is out of tolerance – for example, coated or depleted reference electrode (only for pH sensors; except pH/pNa)
5. If the conductivity sensor is on air (for example in an empty pipe) (only for resistive conductivity sensors)
6. If the conductivity sensor has a short cut (only for resistive conductivity sensors)
7. If no sensor is connected on channel B (only for ISM sensors)
8. If the temperature is out of range, stray light is too high (e.g. because a glass fiber is broken) or the shaft has been removed (see also section 10.1 "Diagnostics"; PATH: Menu/Service/Diagnostics/O₂ optical) (only for optical sensors)
9. If the signal or the temperature value is out of range (see also section 10.1 "Diagnostics"; PATH: Menu/Service/Diagnostics/O₂ optical) (only for optical sensors)
10. If an hardware error has been detected (see also section 10.1 "Diagnostics"; PATH: Menu/Service/Diagnostics/O₂ optical). (only for optical sensors)


11. If the conductivity sensor is on air (for example in an empty pipe) (only for ISM Conductivity sensors)
12. Cell constant (multiplier) is out of tolerance, i.e. has changed too much compared to the value thru the factory calibration (only for ISM conductivity sensors)
13. Electrolyte in the membrane body reaches such a low level that the connection between cathode and reference is disturbed, an immediate action must be taken e.g. exchange and filling the electrolyte.

For 1 and 2 the alarm indicator will be turned off when the alarm message is cleared. It will reappear if the power is constantly cycling or if the watchdog is repeatedly resetting the system.

Only for pH sensors

For 3 and 4 the alarm indicator will go off if the message is cleared and the sensor has been replaced or repaired so that the Rg and Rr values are within specification. If the Rg or Rr message is cleared and Rg or Rr is still out of tolerance then the alarm will stay on and the message will reappear. The Rg and Rr alarm can be turned off by going into this menu and setting Rg diagnostics and/or Rr diagnostics to No. The message can then be cleared and the alarm indicator will be off even though Rg or Rr is out of tolerance.

Pressing the [ENTER] key again will bring up the Save Changes dialog. Selecting No will discard the entered values, selecting Yes will make the entered values the current ones.




Note: There are additional alarms, which will be indicated in the display. See therefore in section 14 "Troubleshooting" the different warning- and alarm lists.

8.3.2 Clean



This menu allows the configuration of clean functionality for the display.

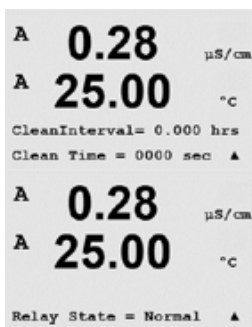

The cleaning interval can be set from 0.000 to 999.9 hours. Setting it to 0 turns the clean cycle off. The cleaning time can be 0 to 9999 seconds and must be smaller than the cleaning interval.

Pressing the [ENTER] key again will bring up the Save Changes dialog. Selecting No will discard the entered values and return to the measurement display screen, selecting Yes will save changes made.



Note: The clean functionality is also available via PROFIBUS PA.

8.4 ISM Set Up (Available for pH, Oxygen and Dissolved Carbon Dioxid ISM Sensors)

(PATH: Menu/Configure/ISM Setup)

Enter Configuration mode as described in section 8.1. "Enter Configuration Mode" and navigate to the menu "ISM set up" by using the ▲ or ▼ key. Press [ENTER]

8.4.1 Sensor Monitoring



Select the menu "Sensor Monitoring" by pressing [ENTER].

The sensor monitoring options can be turned on or off. Via PROFIBUS PA interface you can read out the sensor monitoring values supplied by the Discrete Input Block. The following option is possible:



Lifetime indicator: The dynamic lifetime indication allows an estimation, when the pH electrode or the inner body of an amperometric oxygen sensors is at the end of his lifetime, based on the actual stress he is exposed to. The sensor permanently takes the averaged stress of the past days into consideration and is able to increase/decrease the lifetime accordingly.

Lifetime Indicator	YES/NO
Alarm	YES/NO

The following parameters affect the lifetime indicator:

Dynamic parameters:	Static parameters:
– Temperature	– Calibration history
– pH or oxygen value	– Zero and Slope
– Glass impedance (only pH)	– CIP/SIP/Autoclaving cycles
– Reference impedance (only pH)	

The sensor keeps the information stored in the built in electronics and can be retrieved via a transmitter or the iSense asset management suite.

The alarm will be reset if the Lifetime Indicator is not 0 days anymore (e.g. after connecting a new sensor or changing on the measurement conditions).

For amperometric oxygen sensors, the lifetime indicator is related to the inner-body of the sensor. After exchanging the inner-body, reset the lifetime indicator as described in section 8.4.5 "Reset ISM Counter/Timer".

If the Lifetime Indicator is turned on, in the measuring mode the value will be automatically shown in the display on line 3.

Press [ENTER]



Time to Maintenance: This timer estimates when the next cleaning cycle should be performed to keep the best possible measurement performance. The timer is influenced by significant changes on the DLI parameters.

Time to Maintenance YES/NO
Alarm YES/NO

The time to maintenance can be reset to the initial value by the menu "Reset ISM Counter Timer" (see section 8.4.5 "Reset ISM Counter/Timer"). For amperometric oxygen sensors, the time to maintenance indicates a maintenance cycle for the membrane and electrolyte.

Press [ENTER]




Activation of the **Adaptive Cal Timer:** This timer estimates when the next calibration should be performed to keep the best possible measurement performance. The timer is influenced by significant changes on the DLI parameters.

Adaptive Cal Timer YES/NO
Alarm YES/NO

The Adaptive Calibration Timer will be reset to his initial value after a successful calibration. After a successful calibration will also be the alarm reset. If the Adaptive Cal Timer is turned on, the value will be automatically shown in the display on line 4.

Press [ENTER]




The initial value for Time to Maintenance as well as the Adaptive Calibration Timer can be modified according to the application experience and loaded down to the sensor.




NOTE: By connecting a sensor, the values for Time to Maintenance and/or Adaptive Calibration Timer are read out by the sensor.

Pressing the [ENTER] key again will bring up the Save Changes dialog. Selecting No will discard the entered values and return to the measurement display screen, selecting Yes will save changes made.

8.4.2 CIP Cycle Limit



Navigate to the menu "CIP Cycle Limit" by using the ▲ and ▼ keys and press [ENTER].



The CIP cycle limit counts the number of CIP cycles. If the limit (user defined) is reached, an alarm is shown on the display. Via PROFIBUS PA interface you can read out the CIP Cycle Limit supplied by the Discrete Input Block. The following option is possible:

CIP Max 000	Temp 055
Alarm	YES/NO

If the Max setting is on 000, the counter functionality is turned off. The alarm will be reset after exchanging the sensor. For oxygen sensors, the counter can be reset (see section 8.4.5 "Reset ISM Counter/Timer").

CIP characteristics: CIP Cycles will be automatically recognized by the sensor. Since CIP cycles will vary in intensity (duration and temperature) for each application the algorithm of the counter recognizes an increase of the measurement temperature above a adjustable limit (parameter **Temp** in °C). If the temperature does not decrease below the defined limit within the next 5 minutes after the temperature was reached, the counter in question will be incremented by one and also locked for the next two hours. In the case the CIP would last longer than two hours the counter would be incremented by one once more.

Pressing the [ENTER] key will bring up the Save Changes dialog. Selecting No will discard the entered values, selecting Yes will make the entered values the current ones.

8.4.3 SIP Cycle Limit



Navigate to the menu "SIP Cycle Limit" by using the ▲ and ▼ keys and press [ENTER].



The SIP cycle limit counts the number of SIP cycles. If the limit (user defined) is reached, an alarm can be indicated is shown on the display. Via PROFIBUS PA interface you can read out the SIP Cycle Limit supplied by the Discrete Input Block. The following option is possible:

SIP Max 000	Temp 115
Alarm	YES/NO

If the Max setting is on 000, the counter functionality is turned off. The alarm will be reset after exchanging the sensor. For oxygen sensors, the counter can be reset (see section 8.4.5 "Reset ISM Counter/Timer").


SIP characteristics: SIP Cycles will be automatically recognized by the sensor. Since SIP cycles will vary in intensity (duration and temperature) for each application the algorithm of the counter recognizes an increase of the measurement temperature above a adjustable limit (parameter **Temp** in °C). If the temperature does not decrease below the defined limit within the next 5 minutes after the first temperature was reached, the counter in question will be incremented by one and also locked for the next two hours. In the case the SIP would last longer than two hours the counter would be incremented by one once more.

Pressing the [ENTER] key will bring up the Save Changes dialog. Selecting No will discard the entered values, selecting Yes will make the entered values the current ones.

8.4.4 Autoclaving Cycle Limit



NOTE: The transmitter recognizes the connected ISM sensor and offers this menu only if an auto-clavable sensor is connected.



Navigate to the menu "AutoClave Cycle Limit" by using the ▲ and ▼ keys and press [ENTER].



The Autoclaving Cycle Limit counts the number of autoclaving cycles. If the limit (user defined) is reached, an alarm can be indicated is shown on the display. Via PROFIBUS PA interface you can read out the Autoclaving Cycle Limit supplied by the Discrete Input Block. The following option is possible:

Autoclave Max 000
Alarm YES/NO

If the Max setting is on 000, the counter functionality is turned off. The alarm will be reset after exchanging the sensor. For oxygen sensors, the counter can also be reset manually (see section 8.4.5 "Reset ISM Counter/Timer").

Autoclave characteristics: Since during the autoclaving cycle the sensor is not connected to the transmitter, you will be asked after every sensor connection, whether the sensor was autoclaved or not. According to your selection, the counter will be incremented or not.

Pressing the [ENTER] key will bring up the Save Changes dialog. Selecting No will discard the entered values, selecting Yes will make the entered values the current ones.

8.4.5 Reset ISM Counter/Timer

This menu allows resetting counter and timer functions which cannot be reseted automatically. The adaptive calibration timer will be reseted after a successful adjustment or calibration.

Navigate to the menu "Reset ISM Counter/Timer" by using the ▲ and ▼ keys and press [ENTER].



If an pH sensor or amperometric oxygen sensor is connected, the menu for resetting the Time To Maintenance is displayed. Time To Maintenance needs to be reset after the following operations.

pH sensors: manual maintenance cycle on the sensor.
 oxygen sensor: manual maintenance cycle on the sensor or exchanging of the inner-body or membrane of the sensor


[Press ENTER]



If an oxygen sensor is connected, the menu for resetting the CIP and SIP counter is displayed. These counters should be reset after the following operations.

amperometric sensor: exchanging of the inner-body of the sensor.

[Press ENTER]




8.4.6 DLI Stress Adjustment (Only for pH ISM Sensors)

Through this menu the calculation of the diagnostic data DLI, TTM and ACT can be adapted to application requirements and/or experience.



NOTE: The function is only available for pH ISM sensors with corresponding firmware versions.

Navigate to the menu "DLI Stress Adjustment" by using the ▲ and ▼ keys and press [ENTER].



Adjust the Process Stress parameter based on the particular application and/or requirements

Low: DLI, TTM and ACT will be increased approximately 25% compared with "Medium".
 Medium: Default value, (equal DLI, TTM and ACT values based on former firmware versions of the transmitter).
 High: DLI, TTM and ACT will be reduced approximately 25% compared with "Medium".

Pressing the [ENTER] key will bring up the Save Changes dialog. Selecting No will discard the entered values, selecting Yes will make activate entered values.




8.5 Display

(PATH: Menu/Configure/Display)

Enter configuration mode as described in section 8.1 “Enter Configuration Mode”.

This menu allows for the configuration of the values to be displayed and also the configuration of the display itself.



8.5.1 Measurement


The display has 4 lines. Line 1 on top and Line 4 on the bottom.

Select the values (Measurement a, b, c or d) to be displayed on each line of the display.

The selection of the values for a, b, c, d needs to be done under Configuration/measurement/Channel Setup.



Select the “Error Display” mode. If this is set to “On” when an alarm or warning has occurred, the message “Failure – Press ENTER” will be displayed on Line 4 when an alarm occurs in the normal measurement mode.



Pressing the [ENTER] key again will bring up the Save Changes dialog. Selecting No will discard the entered values, selecting Yes will make the entered values the current ones.




8.5.2 Resolution

This menu allows the setting of the resolution of each displayed value.

The accuracy of the measurement is not effected by this setting.

Possible settings are 1, 0.1, 0.01, 0.001 or Auto.

Pressing the [ENTER] key will bring up the Save Changes dialog.



8.5.3 Backlight



This Menu allows the setting of the back light options of the display.



Possible settings are On, On 50% or Auto Off 50%. If Auto Off 50% is selected then the backlight will go to 50% after 4 minutes with no keypad activity. The backlight will automatically come back on if a key is pressed.

Pressing the [ENTER] key will bring up the Save Changes dialog.

8.5.4 Name



This menu allows for the configuration of an alpha-numeric name which is displayed in the first 9 characters on lines 3 and 4 of the display. The default is nothing (blank).

If a name is entered on line 3 and/or 4 a measurement can be still displayed on the same line.




Use the ◀ and ▶ keys to navigate between digits to be altered. Using the ▲ and ▼ keys to change the character to be displayed. Once all digits of both display channels have been entered, press [ENTER] to bring up the Save Changes dialog.



The resulting display in the measurement mode appears on lines 3 and 4 ahead of the measurements.

8.5.5 ISM Sensor Monitoring (Available When ISM Sensor Connected)



The sensor monitoring allows you to display the sensor monitoring details on line 3 and 4 in the display. The following options are possible:

Line 3 Off/Time Indicator/Time to Maint/Adapt Cal Timer
Line 4 Off/Time Indicator/Time to Maint/Adapt Cal Timer

8.6 Hold Outputs

(PATH: Menu/Configure/Hold Outputs)



Enter configuration mode as described in section 8.1 "Enter Configuration Mode".



The **"Hold outputs"** function applies during the calibration process. If set "Hold outputs" to Yes, during calibration process the corresponding Analog Input of the PROFIBUS PA interface will be at hold state. The hold state depends on the setting. For the possible hold settings, see the list below. The following options are possible:



Hold Outputs? Yes/No

9 System


(PATH: Menu/System)

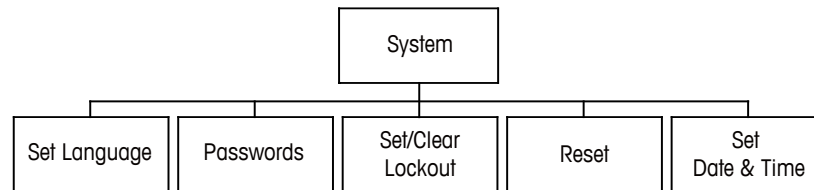


While in measurement mode press the ◀ key. Press the ▼ or ▲ key to navigate to “System” – Menu and press [ENTER].

9.1 Set Language

(PATH: Menu/System/Set Language)



This menu allows the configuration of the display language.




The following selections are possible:
English, French, German, Italian, Spanish, Portuguese, Russian or Japanese (Katakana).


Pressing the [ENTER] key will bring up the Save Changes dialog.

9.2 Passwords

(PATH: Menu/System/Passwords)




This menu allows for the configuration of operator and administrator passwords, as well as setting up a list of allowed menus for the operator. The administrator has rights to access all menus. All default passwords for new transmitters are “00000”.




The passwords menu is protected: Enter the administrator password to enter the menu.

9.2.1 Changing Passwords




See section 9.3 on how to enter the passwords menu. Select Change Administrator or Change Operator and set the new password.




Press the [ENTER] key and confirm the new password. Press [ENTER] again to bring up the Save Changed dialog.

9.2.2 Configuring Menu Access for Operator




See 9.3 on how to enter the passwords Menu. Select Configure Operator to configure the access list for the operator. It is possible to assign/deny rights to the following menus: Cal Key, Quick Setup, Configuration, System, PID Setup and Service.




Choose either Yes or No to give/deny access to the above menus and press [ENTER] to advance to the next items. Pressing the [ENTER] key after configuring all menus will bring up the Save Changes dialog. Selecting No will discard the entered values, selecting Yes will make the entered values the current ones.

9.3 Set/Clear Lockout

(PATH: Menu/System/Set/Clear Lockout)



This menu enables/disables the lockout functionality of the transmitter. The user will be asked for a password before being allowed into any menus if the lockout functionality is enabled.



The lockout-menu is protected: Enter the administrator or operator password and select YES to enable or NO to disable the lockout functionality. Pressing the [ENTER] key after the selection will bring up the Save Changes dialog. Selecting No will discard the entered value, selecting Yes will make the entered value the current one.

9.4 Reset

(PATH: Menu/System/Reset)




NOTE: A reset performed via display, also resets the corresponding PROFIBUS PA parameters to factory default setting. For more information see documentation "PROFIBUS PA parameter Multi-parameter Transmitter M400 PA" on the website "<http://www.mt.com/m400-2wire>".




This menu allows access to the following options:

Reset System, Reset Meter Cal, Reset Analog Cal.

9.4.1 Reset System




This menu allows the reset of the meter to the factory default settings. The meter calibration is not affected.




Pressing the [ENTER] key after the selection will bring up a confirmation screen. Selecting No will return the user to the measurement mode with no changes. Selecting Yes will reset the meter.

9.4.2 Reset Meter Calibration



This menu allows the reset of the meter's calibration factors to the last factory calibration values.



Pressing the [ENTER] key after the selection will bring up a confirmation screen. Selecting No will return the user to the measurement mode with no changes. Selecting Yes will reset the meter calibration factors.

9.5 Set Date & Time





Please enter the actual date and time. The following options are possible. This function is automatically activated at every power-up.

Date (YY-MM-DD):

Time (HH:MM:SS):

10 Service


(PATH: Menu/Service)

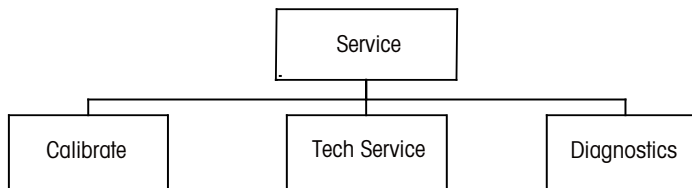

While in measurement mode press the ◀ key. Press the ▲ or ▼ key to navigate to the “Service” menu and press [ENTER]. The available system configuration options are detailed below.


10.1 Diagnostics

(PATH: Menu/Service/Diagnostics)




This menu is a valuable tool for troubleshooting and provides diagnostic functionality for the following items: Model/Software Revision, Display, Keypad, Memory, Read Analog Inputs, O₂ Optical.

10.1.1 Model/Software Revision




Essential information for every Service call is the model and software revision number. This menu shows the part number, model and the serial number of the transmitter. By using the ▼ key it is possible to navigate forward through this menu and get additional information like the current version of firmware implemented on the transmitter: (Master V_XXXX and Comm V_XXXX); and – if an ISM sensor is connected – the version of the sensor firmware (Sensor FW V_XXX) and sensor hardware (Sensor HW XXXX).




Press [ENTER] to exit from this display.

10.1.2 Display




All pixels of the display will be lit for 15 seconds to allow troubleshooting of the display. After 15 seconds the transmitter will return to the normal measuring mode or press [ENTER] to exit sooner.


10.1.3 Keypad




For keypad diagnostics, the display will indicate which key is pressed. Pressing [ENTER] will return the transmitter to the normal measuring mode.



10.1.4 Memory




If Memory is selected then the transmitter will perform a RAM and ROM memory test. Test patterns will be written to and read from all RAM memory locations. The ROM checksum will be recalculated and compared to the value stored in the ROM.



10.1.5 Read Analog Inputs



This menu shows the mA value of the analog input.



Press [ENTER] to exit from this display.

10.1.6 O₂ Optical




This menu shows the state and conditions regarding the optical O₂ sensor. By using the key ▲ or ▼ it is possible to navigate through this menu and get additional information. Press [ENTER] to exit from this display.

10.2 Calibrate

(PATH: Menu/Service/Calibrate)


Enter Service Menu as described in section 10 "Service", select Calibrate, and press [ENTER].

This menu has the options to calibrate the transmitter and the analog inputs and also allows the unlocking of calibration functionality.



10.2.1 Calibrate Meter (Only for Channel A)

The M400 transmitter is factory calibrated within specifications. It is not normally necessary to perform meter re-calibration unless extreme conditions cause an out of spec operation shown by Calibration Verification. Periodic verification/re-calibration may also be necessary to meet Q.A. requirements. Meter calibration can be selected as current (used for most dissolved oxygen, Voltage, Rg Diagnostic, Rr Diagnostic (used for pH), and temperature (used for all measurements).



10.2.1.1 Resistance

The meter is equipped with five (5) internal ranges of measurement on each channel. Each resistance range and temperature is calibrated separately, with each resistance range consisting of a two-point calibration.

Below is a table showing the resistance values for all calibration ranges.


Range	Point 1	Point 2	Point 4
Resistivity 1	1.0 Mohms	10.0 Mohms	–
Resistivity 2	100.0 Kohms	1.0 Mohms	–
Resistivity 3	10.0 Kohms	100.0 Kohms	–
Resistivity 4	1.0 Mohms	10.0 Kohms	–
Resistivity 5	100 Ohms	1.0 Mohms	–
Temperature	1000 Ohms	3.0 Kohms	66 Kohms

It is recommended that both calibration and verification be performed using the M400 Calibrator Module Accessory (refer to accessory list, in section 15). Instructions on the use of this accessory are provided with the calibrator module.




Navigate to the Calibrate Meter screen and select Channel A or B, and Resistance 1, designating that the transmitter is ready to calibrate the first range resistor. This resistance may be changed, selecting range 1 thru 5. Each resistance range consists of a two-point calibration.

Press [ENTER] to begin the calibration process.




The first text line will ask for the Point 1 resistance value (this will correspond to Resistance 1 value shown on the Calibration Module Accessory). The second text line will show the measured resistance value. When the value stabilizes, press [ENTER] to perform calibration.




The transmitter screen will then prompt the user to enter the value for Point 2, and R1 will display the measured resistance value. When this value stabilizes, press [ENTER] to calibrate this range and bring up a confirmation screen.

Select Yes to save the calibration values and the successful Calibration is confirmed on the display. The transmitter will return to the Measurement mode in approximately 5 seconds.



Once point 1 and 2 are calibrated, return to the Calibrate Meter screen. Move the cursor to change to Resistance 2, designating the second calibration range. Proceed with the two-point calibration process as performed for the first range. This same process must be followed to complete the resistance calibration of all 5 ranges.


10.2.1.2 Temperature



Temperature is performed as a three point calibration. The table above shows the resistance values of these three points.

Navigate to the Calibrate Meter screen and choose Temperature calibration for Channel A.

Press [ENTER] to begin temperature calibration process.





The first text line will ask for the Point 1 temperature resistance value (this will correspond to temperature 1 value shown on the calibration module accessory). The second text line will show the measured resistance value. When the value stabilizes, press [ENTER] to perform calibration.

The transmitter screen will then prompt the user to enter the value for Point 2, and T2 will display the measured resistance value. When this value stabilizes, press [ENTER] to calibrate this range.


Repeat these steps for Point 3.

Press [ENTER] to bring up a confirmation screen. Select Yes to save the calibration values and the successful calibration is confirmed on the display.

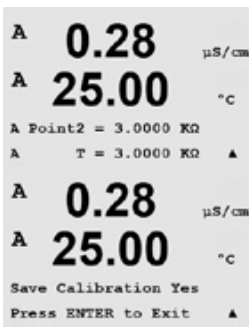


The transmitter will return to the measurement mode in approximately 5 seconds.

10.2.1.3 Current




Current calibration is performed as a two-point calibration.

Navigate to the Calibrate Meter screen and select Channel A.

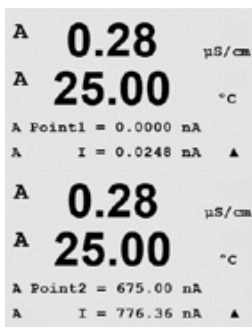

Enter the value for Point 1, in milliamps, of the current source connected to the input. The second display line will show the measured current. Press [ENTER] to begin the calibration process.




Enter the value for Point 2, in milliamps, of the current source connected to the input. The second display line shows the measured current.

Pressing the [ENTER] key after entering Point 2 will bring up a confirmation screen. Select Yes to save the calibration values and the successful calibration is confirmed on the display. The transmitter will return to the measurement mode in approximately 5 seconds.




Note: Depending on the range of the measured current of the connected oxygen sensor, select the input range which has to be calibrated. Select Current1 for an input signal 0 to approx. –750 nA and Current2 for an input signal 0 to approx. –7500 nA.

10.2.1.4 Voltage




Voltage calibration is performed as a two-point calibration.


Navigate to the Calibrate Meter screen and select Channel A and Voltage.



Enter the value for Point 1 in, volts, connected to the input. The second display line will show the measured voltage. Press [ENTER] to begin the calibration process.




Enter the value for Point 2, in volts, of the source connected to the input. The second display line shows the measured voltage.




Pressing the [ENTER] key after entering Point 2 will bring up a confirmation screen. Select Yes to save the calibration values and the successful Calibration is confirmed on the display. The transmitter will return to the measurement mode in approximately 5 seconds.


10.2.1.5 Rg Diagnostic




Rg diagnostic is performed as a two-point calibration. Navigate to the Calibrate Meter screen and select Channel A and Rg Diagnostic.



Enter the value for Point 1 of the calibration according to the resistor connected across the pH glass electrode measuring input. Press [ENTER] to begin the calibration process.




Enter the value for Point 2 of the calibration according to the resistor connected across the pH glass electrode measuring input.




Pressing the [ENTER] key after entering Point 2 will bring up a confirmation screen. Select Yes to save the calibration values and the successful calibration is confirmed on the display. The transmitter will return to the measurement mode in approximately 5 seconds.

10.2.1.6 Rr Diagnostic




Rr diagnostic is performed as a two-point calibration. Navigate to the Calibrate Meter screen and select Channel A and Rr Diagnostic.



Enter the value for Point 1 of the calibration according to the resistor connected across the pH reference measuring input. Press [ENTER] to begin the calibration process.




Enter the value for Point 2 of the calibration according to the resistor connected across the pH reference measuring input.




Pressing the [ENTER] key after entering Point 2 will bring up a confirmation screen. Select Yes to save the calibration values and the successful calibration is confirmed on the display. The transmitter will return to the measurement mode in approximately 5 seconds.

10.2.1.7 Calibrate Analog Input Signal




The analog input can be calibrated at two current values e.g. 4 mA and 20 mA.




Connect an accurate milliamp meter to the analog input terminals. Enter the value for Point 1, e.g. 4 mA value. The second line shows the measured current.

Press [Enter] to go on.




Enter the value for Point 2, e.g. 20 mA value




Pressing the [ENTER] key after entering Point 2 will bring up a confirmation screen. Selecting No will discard the entered values, selecting Yes will make the entered values the current ones.

10.2.2 Calibrate Unlock



Select this Menu to configure the CAL Menu, see section 7.



Selecting Yes means that meter calibration menus will be selectable under the CAL Menu. Selecting No means that only the sensor calibration is available under the CAL Menu. Press [ENTER] after the selection to display a confirmation screen.

10.3 Tech Service


(PATH: Menu/Tech Service)




Note: This menu is for METTLER TOLEDO service personnel use only.

11 Info

(PATH: Info)

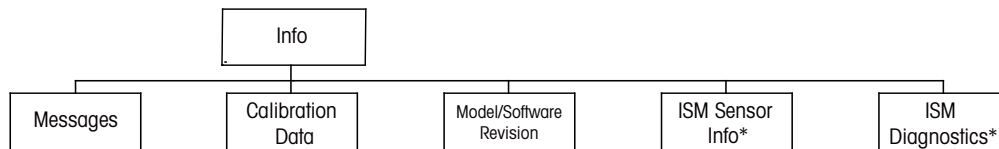


* Only available in combination with ISM sensors




Pressing the ▼ key will display the Info menu with the options Messages, Calibration Data and Model/Software Revision.

11.1 Messages

(PATH: Info/Messages)



The most recent message is displayed. The up and down arrow keys allow scrolling through the last four messages that have occurred.



Clear Messages clears all the messages. Messages are added to the message list when the condition that generates the message first occurs. If all messages are cleared and a message condition still exists and started before the clear then it will not appear in the list. For this message to re-occur in the list the condition must go away and then reappear.

Press [ENTER] to exit from this display.

11.2 Calibration Data

(PATH: Info/Calibration Data)



Selecting Calibration Data displays the calibration constants for each sensor.




P = calibration constants for the primary measurement
S = calibration constants for the secondary measurement

Press ▼ for ORP calibration data of ISM pH sensors.

Press [ENTER] to exit from this display.


11.3 Model/Software Revision

(PATH: Info/Model/Software Revision)



Selecting Model/Software Revision will display the part number, model and the serial number of the transmitter.

By using the ▼ key it is possible to navigate forward through this menu and get additional information like the current version of firmware implemented on the transmitter (Master V_XXXX and Comm V_XXXX) and – if an ISM sensor is connected – the version of the sensor firmware (Sensor FW V_XXX) and sensor hardware (Sensor HW XXXX).



The displayed information is important for any Service call. Press [ENTER] to exit from this display.


11.4 ISM Sensor Info (Available when ISM Sensor Connected)

(PATH: Info/ISM Sensor Info)



After plugging in an ISM sensor it is possible by using the key ▲ or ▼ to navigate to the Menu "ISM Sensor Info".

Press [ENTER] to select the menu.



The following information about the sensor will be shown in this menu. Use up and down arrows to scroll in the menu. Type: Type of sensor (e.g. InPro 3250)

Cal Date: Date of the last adjustment


Serial-No.: Serial number of the connected sensor

Part-No.: Part number of the connected sensor

Press [ENTER] to exit from this display.

11.5 ISM Sensor Diagnostics (Available when ISM Sensor Connected)

(PATH: Info/ISM Diagnostics)



After plugging in an ISM sensor it is possible by using the key ▲ or ▼ to navigate to the Menu "ISM Diagnostics".

Press [ENTER] to select the menu.

Navigate to one of the menus, described in this section, and press [ENTER] again.



Cal History

The calibration history is stored with a time stamp in the ISM sensor and is displayed on the transmitter. The calibration history offers the following information:

Fact (Factory calibration): This is the original dataset, determined in the factory. This dataset remains stored in the sensor for reference and cannot be overwritten.

Act (Actual adjustment): This is the actual calibration dataset which is used for the measurement. This dataset moves to Cal2 position after the next adjustment.

1. Adj (First adjustment): This is the first adjustment after the factory calibration. This dataset remains stored in the sensor for reference and cannot be overwritten

Cal1 (last calibration/adjustment): This is the last executed calibration/adjustment. This dataset moves to Cal2 and then to Cal3 when a new calibration/adjustment is performed. Afterwards, the dataset is not available anymore.

Cal2 and Cal3 acting in the same way as Cal1.

Definition:

Adjustment: The calibration procedure is completed and the calibration values are taken over and used for the measurement (Act) and stated in Cal1. The current values from Act will move to Cal2.


Calibration: The calibration procedure is completed, but the calibration values will not be over-taken and the measurement continuous with the last valid adjustment dataset (Act). The dataset will be stored under Cal1.

The calibration history is used for the estimation of the lifetime indicator for ISM sensors.

Press [ENTER] to exit from this display.




Note: This function requires the correct setting of date and time during calibration and/or adjustment tasks (see section 9.5 "Set Date & Time").




Sensor monitoring (not available for Cond 4-e sensor)

The sensor monitoring shows the different diagnostics functions available for each ISM sensor. The following information is available:



Lifetime Indicator: Shows an estimation of the remaining lifetime to ensure a reliable measurement. The lifetime is indicated in days (d) and percentage (%). For a description of the Lifetime indicator, please see section 8.4 "ISM Set Up (Available for pH, Oxygen and Dissolved Carbon Dioxid ISM Sensors)". For oxygen sensors, the lifetime indicator is related to the inner-body of the sensor. If you want to bring the bar indicator on the screen, see section 8.4 to activate ISM functions.




Adaptive Cal Timer: This timer shows a Adaptive Cal Timer, when the next calibration should be performed to keep the best possible measurement performance. The Adaptive Cal Timer is indicated in days (d) and percentage (%). For a description of the Adaptive Cal Timer, please see section 8.4.



Time to Maintenance: This timer shows a Time to Maintenance, when the next cleaning cycle should be performed to keep the best possible measurement performance. The Time to Maintenance is indicated in days (d) and percentage (%). For a description of the Time to Maintenance, please see section 8.4. For oxygen sensors, the Time to Maintenance indicates a maintenance cycle for the membrane and electrolyte.

Press [ENTER] to exit from this display.



Max. Temperature

The maximum temperature shows the maximum temperature that this sensor has ever seen, together with a time stamp of this maximum. This value is stored on the sensor and cannot be changed. During autoclaving the Max temperature is not recorded.

Max. Temperature

Tmax XXX°CYY/MM/DD

Press [ENTER] to exit from this display.



Note: This function requires the correct setting of date and time of the transmitter, (see section "9.5 "Set Date & Time")



CIP Cycles

Shows the amount of CIP cycles that the sensor has been exposed to. For a description of the CIP Cycle indicator, please see section 8.4.

CIP Cycles xxx of xxx

Press [ENTER] to exit from this display.



SIP Cycles

Shows the amount of SIP cycles that the sensor has been exposed to. For a description of the SIP Cycle indicator, please see section 8.4.

SIP Cycles xxx of xxx

Press [ENTER] to exit from this display.



Autoclaving Cycles

Shows the amount of Autoclaving cycles that the sensor has been exposed to. For a description of the AutoClave Cycle indicator, please see section 8.4.

Autoclaving Cycles xxx of xxx


Press [ENTER] to exit from this display.

12 PROFIBUS PA Interface

12.1 General

12.1.1 System Architecture

The following diagram shows typical examples of a PROFIBUS PA network with the associated components.

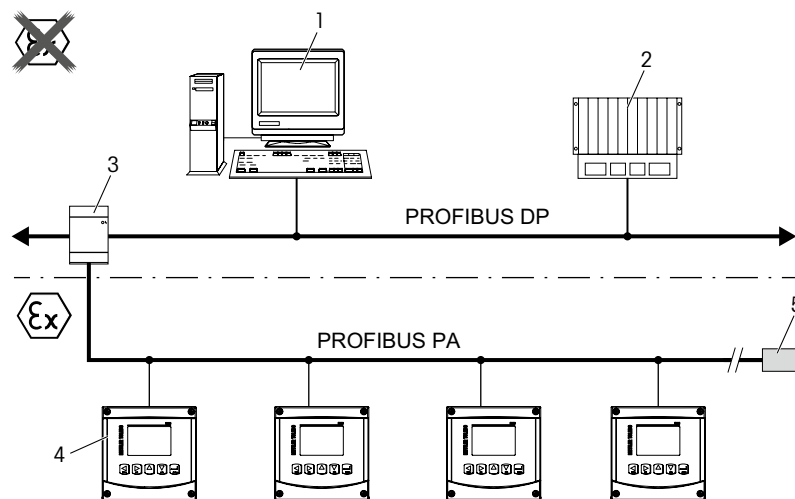

- 1 PC with PROFIBUS interface card and PROFIBUS configuration program (Class 2 master)
- 2 PLC (Class 1 master)
- 3 Segment coupler DP/PA
- 4 M400 PA transmitter with connected sensor (sensor not illustrated)
- 5 PROFIBUS PA terminating resistor



NOTE: Further information on PROFIBUS PA can be found in the PNO Guideline and standards IEC 61158, IEC 61784, EN 50170/DIN 19245 and EN 50020 (FISCO model).

12.2 M400 PA Block Model

With PROFIBUS PA, all the instrument parameters are categorized according to their functional properties and task and are generally assigned to three different blocks.

A PROFIBUS PA instrument has the following block types:

A Resource Block (device block)

This block contains all the device-specific features of the device.

One Analyser transducer block (sensor block)

The "Sensor Block " contains the measuring principles and the sensor-specific parameters.

One or more function blocks


Function blocks contain the automation functions of the instrument. There are different function blocks such as the Analog Input Block or Discrete Input Block. Each of these function blocks is used to execute different application functions.

The function blocks can be connected by means of an PROFIBUS configuration program, depending on the automation task.

M400 PA contains the following blocks:

- 1 Resource Block (device block)
- 1 Analyser Transducer Block (sensor block)
- 9 Function Blocks: 4 Analog Input Blocks (AI), 1 Analog Output Block (AO), 2 Discrete Input Block (DI), 2 Discrete Output Block (DO)

12.2.1 Block Configuration

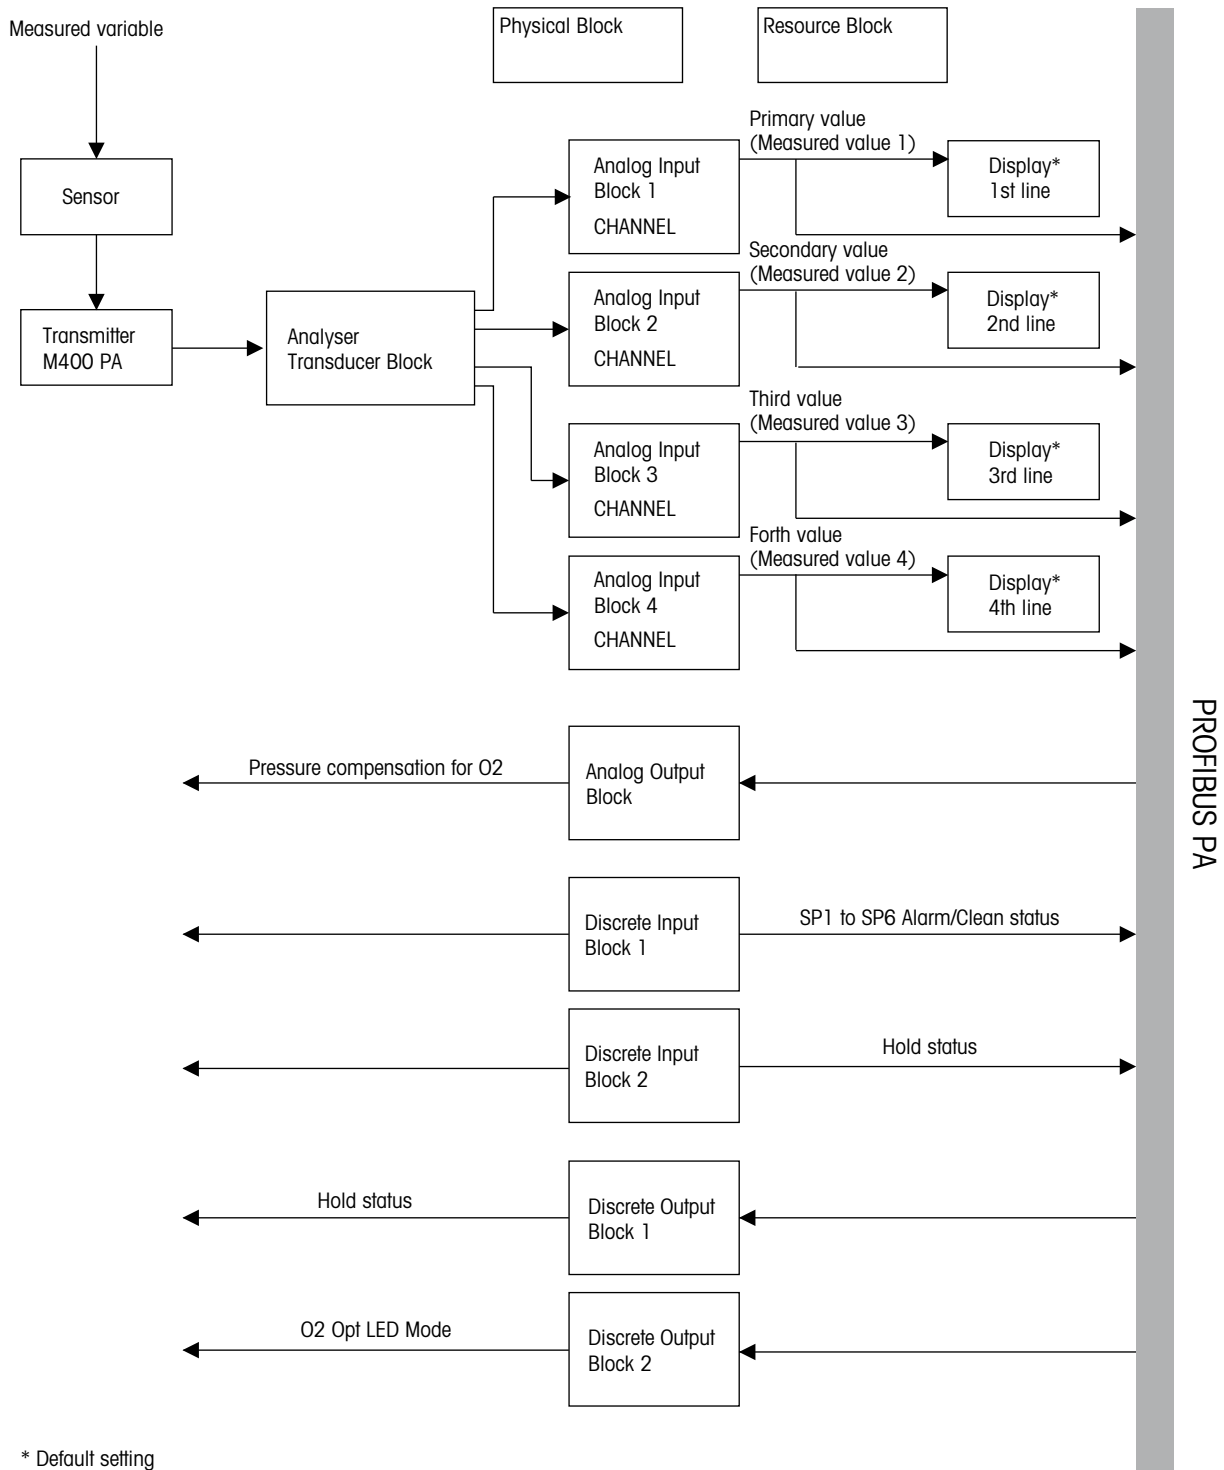

* Default setting



NOTE: If a reset by means of the RESTART parameter, "Default" option in the Resource Block is performed, the links between the blocks are deleted and the PROFIBUS PA parameters are reset to the default values.

12.3 Commissioning

12.3.1 Network Configuration

1. Copy the GSD file into the GSD-directory of the configuration program.
GSD file: METTOE8A.gsd
2. Update hardware catalogue.
3. Integrate M400 PA transmitter into the DP master system.
4. Set PROFIBUS address for M400.
5. Factory setting: 126, Input range: 0 ... 125.
6. Perform parameterization either via display on-site or via a PROFIBUS configuration program.

Upon successful integration of the M400 PA transmitter in the PROFIBUS system, the symbol "PA" appears on the display.



NOTE: For further information on integrating the instrument into the PROFIBUS system, see the description for the configuration software used. For step 1 to 4 see documentation of the configuration program.

12.3.2 Set PROFIBUS address

Every PROFIBUS participant must have a unique address assigned for communication.

The address "126" set in the factory may be used for function testing of the instrument and for connection to a PROFIBUS network in operation. Then you may change this address to integrate other devices.

You may change the PROFIBUS address via a PROFIBUS configuration program.

12.3.3 Device Master File (GSD file)

To integrate the field devices into the bus system, the PROFIBUS PA system requires a description of the device such as device identification, ID number, supported communication features, module structure (combination of cyclic input and output telegrams) and meaning of diagnosis bits. These data are contained in a Device Master File (GSD file). Device bitmaps, which appear as icons in the network tree, can also be integrated.

The GSD file and the corresponding bitmaps are required for projecting of a PROFIBUS-DP network. Every instrument receives an ID number by the PROFIBUS user organization (PNO). The name of the GSD file is derived from this.

The following versions of GSD are possible when using devices that support the "PA devices" profile:

- Manufacturer-specific GSD, ID number: 0x0E8A (factory setting):
This GSD guarantees the unlimited functionality of the field device. All device-specific process parameters and functions are available.
- Profile GSD:
As an alternative to the manufacturer-specific GSD, the PNO makes a general database file available with the name PA139750.gsd.

Name	Comments	ID number	GSD	Bitmap
M400 PA	Manufacturer-specific GSD	0x0E8A	METTOE8A.gsd	METTOE8A.bmp
	Profile GSD	0x9750	PA139750.gsd	–

The GSD file is provided on the supplied CD-ROM "METTLER TOLEDO M400 PA Transmitter Series, Operation Documentation".

The files for M400 FF can also be acquired as follows:

- Internet METTLER TOLEDO: <http://www.mt.com/m400-2wire>
- Internet PNO: <http://www.profibus.com>

13 Maintenance

13.1 Front Panel Cleaning

Clean the front panel with a damp soft cloth (water only, no solvents). Gently wipe the surface and dry with a soft cloth.

14 Troubleshooting

If the equipment is used in a manner not specified by METTLER TOLEDO the protection provided by the equipment may be impaired. Review the table below for possible causes of common problems:

Problem	Possible Cause
Display is blank.	<ul style="list-style-type: none"> – No power to M400. – LCD display contrast set incorrectly. – Hardware failure.
Display does not show "PA" symbol. When the connection to the PROFIBUS system has been built up, the "PA" symbol is shown. The transmitter has to be in measurement mode.	<ul style="list-style-type: none"> – Incorrect wiring of the transmitter. – An incorrect bus address for the transmitter is set. – Incorrect integration of the transmitter in the PROFIBUS system.
Incorrect measurement readings.	<ul style="list-style-type: none"> – Sensor improperly installed. – Incorrect units multiplier entered. – Temperature compensation incorrectly set or disabled. – Sensor or transmitter needs calibration. – Sensor or patch cord defective or exceeds recommended maximum length. – Hardware failure.
Measurement readings not stable.	<ul style="list-style-type: none"> – Sensors or cables installed too close to equipment that generates high level of electrical noise. – Recommended cable length exceeded. – Averaging set too low. – Sensor or patch cord defective.
Displayed Δ is flashing.	<ul style="list-style-type: none"> – Setpoint is in alarm condition (setpoint exceeded). – Alarm has been selected (see section 8.3.1 "Alarm") and occurred.
Cannot change menu settings.	<ul style="list-style-type: none"> – User locked out for security reasons.

14.1 Cond (resistive) Error Messages / Warning- and Alarm List for Analog Sensors

Alarms	Description
Watchdog time-out*	SW/System fault
Cond Cell open*	Cell running dry (no measurement solution) or wires are broken
Cond Cell shorted*	Short circuit caused by sensor or cable

* According to the parameterization of the transmitter (see section 8.3.1 "Alarm"; PATH: Menu/Configure/Alarm/Clean/Setup Alarm)

14.2 Cond (resistive) Error Messages / Warning- and Alarm List for ISM Sensors

Alarms	Description
Watchdog time-out*	SW/System fault
Dry Cond sensor*	Cell running dry (no measurement solution)
Cell deviation*	Multiplier out of tolerance** (depends on sensor model).

* According to the parameterization of the transmitter (see section 8.3.1 "Alarm";
PATH: Menu/Configure/Alarm/Clean/Setup Alarm)

** For further information refer to the sensor documentation

14.3 pH Error Messages/Warning- and Alarm List

14.3.1 pH Sensors except Dual Membrane pH Electrodes

Warnings	Description
Warning pH slope >102%	Slope too big
Warning pH Slope <90%	Slope too small
Warning pH Zero \pm 0.5 pH	Out of range
Warning pHGs change <0.3**	Glass electrode resistance changed by more than factor 0.3
Warning pHGs change >3**	Glass electrode resistance changed by more than factor 3
Warning pHRef change <0.3**	Reference electrode resistance changed by more than factor 0.3
Warning pHRef change >3**	Reference electrode resistance changed by more than factor 3

Alarms	Description
Watchdog time-out*	SW/System fault
Error pH Slope >103%	Slope too big
Error pH Slope <80%	Slope too small
Error pH H Zero \pm 1.0 pH	Out of range
Error pH Ref Res >150 K Ω **	Reference electrode resistance too big (break)
Error pH Ref Res <2000 Ω **	Reference electrode resistance too small (short)
Error pH Gls Res >2000 M Ω **	Glass electrode resistance too big (break)
Error pH Gls Res <5 M Ω **	Glass electrode resistance too small (short)

* ISM sensors only

** According to the parameterization of the transmitter (see section 8.3.1 "Alarm";
PATH: Menu/Configure/Alarm/Clean/Setup Alarm)

14.3.2 Dual Membrane pH Electrodes (pH/pNa)

Warnings	Description
Warning pH slope >102%	Slope too big
Warning pH Slope <90%	Slope too small
Warning pH Zero \pm 0.5 pH	Out of range
Warning pHGs change <0.3*	Glass electrode resistance changed by more than factor 0.3
Warning pHGs change >3*	Glass electrode resistance changed by more than factor 3
Warning pNaGs change<0.3*	Glass electrode resistance changed by more than factor 0.3
Warning pNaGs change >3*	Reference electrode resistance changed by more than factor 3

Alarms	Description
Watchdog time-out	SW/System fault
Error pH Slope >103%	Slope too big
Error pH Slope <80%	Slope too small
Error pH pH Zero \pm 1.0 pH	Out of range
Error pNa Gls Res > 2000 M Ω *	Glass electrode resistance too big (break)
Error pNa Gls Res < 5 M Ω *	Glass electrode resistance too small (short)
Error pH Gls Res > 2000 M Ω *	Glass electrode resistance too big (break)
Error pH Gls Res < 5 M Ω *	Glass electrode resistance too small (short)

* According to the parameterization of the transmitter (see section 8.3.1 "Alarm";
PATH: Menu/Configure/Alarm/Clean/Setup Alarm)

14.3.3 ORP Messages

Warnings*	Description
Warning ORP ZeroPt >30 mV	Zero offset too big
Warning ORP ZeroPt <-30 mV	Zero offset too small

Alarms*	Description
Watchdog time-out	SW/System fault
Error ORP ZeroPt >60 mV	Zero offset too big
Error ORP ZeroPt <-60 mV	Zero offset too small

* ISM sensors only

14.4 Amperometric O₂ Error Messages/Warning- and Alarm List

14.4.1 High Level Oxygen Sensors

Warnings	Description
Warning O ₂ Slope < -90 nA	Slope too big
Warning O ₂ Slope > -35 nA	Slope too small
Warning O ₂ ZeroPt > 0.3 nA	Zero offset too big
Warning O ₂ ZeroPt < -0.3 nA	Zero offset too small

Alarms	Description
Watchdog time-out*	SW/System fault
Error O ₂ Slope < -110 nA	Slope too big
Error O ₂ Slope > -30 nA	Slope too small
Error O ₂ ZeroPt > 0.6 nA	Zero offset too big
Error O ₂ ZeroPt < -0.6 nA	Zero offset too small
Electrolyte Low*	Too low level of electrolyte

* ISM sensors only

14.4.2 Low Level Oxygen Sensors

Warnings	Description
Warning O ₂ Slope < -460 nA	Slope too big
Warning O ₂ Slope > -250 nA	Slope too small
Warning O ₂ ZeroPt > 0.5 nA	Zero offset too big
Warning O ₂ ZeroPt < -0.5 nA	Zero offset too small

Alarms	Description
Watchdog time-out*	SW/System fault
Error Install O ₂ Jumper	In case of using InPro 6900 a jumper has to be installed (see section 4.3.5 "TB2 – pH, Amp. Oxygen, Ozone, Conductivity 4-e and Dissolved CO ₂ (Low) ISM (Digital) Sensors").
Error O ₂ Slope < -525 nA	Slope too big
Error O ₂ Slope > -220 nA	Slope too small
Error O ₂ ZeroPt > 1.0 nA	Zero offset too big
Error O ₂ ZeroPt < -1.0 nA	Zero offset too small
Electrolyte Low*	Too low level of electrolyte

* ISM sensors only

14.4.3 Trace Oxygen Sensors

Warnings	Description
Warning O ₂ Slope < -5000 nA	Slope too big
Warning O ₂ Slope > -3000 nA	Slope too small
Warning O ₂ ZeroPt > 0.5 nA	Zero offset too big
Warning O ₂ ZeroPt < -0.5 nA	Zero offset too small

Alarms	Description
Watchdog time-out	SW/System fault
Error O ₂ Slope < -6000 nA	Slope too big
Error O ₂ Slope > -2000 nA	Slope too small
Error O ₂ ZeroPt > 1.0 nA	Zero offset too big
Error O ₂ ZeroPt < -1.0 nA	Zero offset too small
Electrolyte Low*	Too low level of electrolyte

* ISM sensors only

14.5 Optical O₂ Error Messages/Warning- and Alarm List

Warnings	Description
Chx Cal Required*	ACT = 0 or measured values out of range
Chx CIP Counter Expired	Limit of CIP cycles reached
Chx SIP Counter Expired	Limit of SIP cycles reached
Chx Autocl. Count. Exp.	Limit of autoclaving cycles reached

* If this warning is displayed, you will find more information about the cause for the warning in Menu/Service/Diagnostics/O₂ optical

Alarms	Description
Watchdog time-out	SW/System fault
Chx Signal error**	Signal or value for temperature out of range
Chx Shaft error**	Temperature bad or stray light too high (e.g. because a glass is fiber broken) or shaft has been removed
Chx Hardware error**	Electronic components fail

** According to the parameterization of the transmitter (see section 8.3.1 "Alarm";
PATH: Menu/Configure/Alarm/Clean/Setup Alarm)

If an alarm has occurred, you will find more information about the cause for the alarm in Menu/Service/Diagnostics/O₂ optical

14.6 Dissolved Carbon Dioxide Error Messages/ Warning- and Alarm List

Warnings	Description
Warning pH slope >102%	Slope too big
Warning pH Slope <90%	Slope too small
Warning pH Zero \pm 0.5 pH	Out of range
Warning pHGs change <0.3*	Glass electrode resistance changed by more than factor 0.3
Warning pHGs change >3*	Glass electrode resistance changed by more than factor 3

Alarms	Description
Watchdog time-out*	SW/System fault
Error pH Slope >103%	Slope too big
Error pH Slope <80%	Slope too small
Error pH Zero \pm 1.0 pH	Out of range
Error pH Gls Res >2000 M Ω *	Glass electrode resistance too big (break)
Error pH Gls Res <5 M Ω *	Glass electrode resistance too small (short)

* According to the parameterization of the transmitter (see section 8.3.1 "Alarm";
PATH: Menu/Configure/Alarm/Clean/Setup Alarm).

14.7 Thermal conductivity CO₂ sensor/Warning- and alarm messages

Warnings	Description
ChX error CO ₂ slope > xx mV	Slope to big
ChX error CO ₂ slope < yy mV	Slope to small
ChX BL out of range	Baseline out of range (purge gas, membrane or electronics failure)

Alarms	Description
ChX CO ₂ overrange	CO ₂ raw signal in overrange
ChX CO ₂ underrange	CO ₂ raw signal in underrange
ChX Temp. overrange	Temperature overrange
ChX Temp. underrange	Temperature underrange
ChX TC-sensor cut off	Measurement of TC-sensor is interrupted (for protective reasons)
ChX board error	Electronic component failure
CHX TC-sensor fail	Thermal conductivity sensor failure
CHX valve open	Purge gas valve permanently open
ChX SW error	Software error
ChX membrane error	membrane error
ChX not connected	Sensor not connected
ChX Temp. not reliable	Temperature reading not reliable
ChX CO ₂ not reliable	CO ₂ readings not reliable

14.8 Warning- and Alarm Indication on the Display

14.8.1 Warning Indication

If there are conditions, which generate a warning, the message will be recorded and can be selected through the menu Messages (PATH: Info/Messages; see also section 11.1 "Messages"). According to the configuration of the transmitter the hint "Failure – Press ENTER" will be shown at line 4 of the display, if a warning or alarm has occurred (see also section 8.5 "Display"; PATH: Menu/Configure/Display/Measurement).

14.8.2 Alarm Indication

Alarms will be shown in the display by a flashing symbol Δ and recorded through the menu point Messages (PATH: Info/Messages; see also section 11.1 "Messages").

Furthermore the detection of some alarms can be activated or deactivated (see section 8.3 "Alarm/Clean"; PATH: Menu/Configure/Alarm/Clean) for an indication on the display. If one of these alarms occurs and the detection has been activated, the flashing symbol Δ will be shown on the display and the message will be recorded through the menu Messages (see section 11.1 "Messages"; PATH: Info/Messages).

According to the parameterisation of the transmitter the hint "Failure – Press ENTER" will be shown at line 4 of the display, if a warning or alarm has occurred (see also section 8.5 "Display"; PATH: Menu/Configure/Display/Measurement).

15 Accessories and Spare Parts

Please contact your local METTLER TOLEDO sales office or representative for details for Additional accessories and spare parts.

Description	Order no.
Pipe Mount Kit for ½ DIN models	30 300 480
Panel Mount Kit for ½ DIN models	52 500 213
Protective Hood for ½ DIN models	30 073 328

16 Specifications

16.1 General Specifications

Conductivity 2-e/4-e

Measurement parameters	Conductivity/resistivity and temperature
Conductivity ranges	0.02 to 2,000 $\mu\text{S}/\text{cm}$ (500 $\Omega \times \text{cm}$ to 50 $\text{M}\Omega \times \text{cm}$)
2-electrode sensor	C = 0.01 0.002 to 200 $\mu\text{S}/\text{cm}$ (5000 $\Omega \times \text{cm}$ to 500 $\text{M}\Omega \times \text{cm}$)
	C = 0.1 0.02 to 2000 $\mu\text{S}/\text{cm}$ (500 $\Omega \times \text{cm}$ to 50 $\text{M}\Omega \times \text{cm}$)
	C = 1 15 to 4000 $\mu\text{S}/\text{cm}$
	C = 3 15 to 12,000 $\mu\text{S}/\text{cm}$
	C = 10 10 to 40,000 $\mu\text{S}/\text{cm}$ (25 $\Omega \times \text{cm}$ to 100 $\text{k}\Omega \times \text{cm}$)
Conductivity ranges	0.01 to 650 mS/cm (1.54 $\Omega \times \text{cm}$ to 0.1 $\text{M}\Omega \times \text{cm}$)
4-electrode sensor	
Display range for 2-e sensor	0 to 40,000 mS/cm (25 $\Omega \times \text{cm}$ to 100 $\text{M}\Omega \times \text{cm}$)
Display range for 4-e sensor	0.01 to 650 mS/cm (1.54 $\Omega \times \text{cm}$ to 0.1 $\text{M}\Omega \times \text{cm}$)
Chemical concentration curves	NaCl: 0–26% @ 0 °C to 0–28% @ +100 °C NaOH: 0–12% @ 0 °C to 0–16% @ +40 °C to 0–6% @ +100 °C HCl: 0–18% @ –20 °C to 0–18% @ 0 °C to 0–5% @ +50 °C HNO ₃ : 0–30% @ –20 °C to 0–30% @ 0 °C to 0–8% @ +50 °C H ₂ SO ₄ : 0–26% @ –12 °C to 0–26% @ +5 °C to 0–9% @ +100 °C H ₃ PO ₄ : 0–35% @ +5 °C to +80 °C User-defined concentration table (5 × 5 matrix)
TDS ranges	NaCl, CaCO ₃
Cond/Res accuracy ¹⁾	Analog: $\pm 0.5\%$ of reading or 0.25 Ω , whichever is greater, up to 10 $\text{M}\Omega\text{-cm}$
Cond/Res repeatability ¹⁾	Analog: $\pm 0.25\%$ of reading or 0.25 Ω , whichever is greater
Cond/Res resolution	Auto/0.001/0.01/0.1/1 (can be selected)
Temperature input	Pt1000/Pt100/NTC22K
Temperature measuring range	–40 to +200 °C (–40 to +392 °F)
Temperature resolution	Auto/0.001/0.01/0.1/1 (can be selected)
Temperature accuracy	– ISM: ± 1 digit – Analog: ± 0.25 °C (± 32.5 °F) within –30 to +150 °C (–22 to +302 °F); ± 0.50 °C (± 32.9 °F) outside
Temperature repeatability ¹⁾	± 0.13 °C (± 32.2 °F)
Max. sensor cable length	– ISM: 80 m (260 ft) – Analog: 61 m (200 ft); with 4-e sensors: 15 m (50 ft)
Calibration	1-point, 2-point or process

1) ISM input signal causes no additional error.

pH/ORP

Measurement parameters	pH, mV and temperature
pH display range	-2.00 to +20.00 pH
pH resolution	Auto/0.001/0.01/0.1/1 (can be selected)
pH accuracy ¹⁾	Analog: ± 0.02 pH
mV range	-1500 to +1500 mV
mV resolution	Auto/0.001/0.01/0.1/1 mV (can be selected)
mV accuracy ¹⁾	Analog: ± 1 mV
Temperature input ²⁾	Pt1000/Pt100/NTC30K
Temperature measuring range	-30 to 130 °C (-22 to 266 °F)
Temperature resolution	Auto/0.001/0.01/0.1/1 (can be selected)
Temperature accuracy ¹⁾	Analog: ± 0.25 °C in the range of -10 to +150 °C (± 32.5 °F in the range of +14 to +176 °F)
Temperature repeatability ¹⁾	± 0.13 °C (± 32.2 °F)
Temperature compensation	Automatic/Manual
Max. sensor cable length	- Analog: 10 to 20 m (33 to 65 ft) depending on sensor - ISM: 80 m (260 ft)
Calibration	1-point (offset), 2-point (slope or offset) or process (offset)

1) ISM input signal causes no additional error.

2) Not required on ISM sensors

Available Buffer Sets

Standard buffers	MT-9 buffers, MT-10 buffers, NIST Technical Buffers, NIST Standard Buffers (DIN 19266:2000-01), JIS Z 8802 buffers, Hach buffers, CIBA (94) buffers, Merck Titrisols-Reidel Fixanals, WTW buffers
Dual membrane electrode pH buffers (pH/pNa)	Mettler-pH/pNa buffers (Na+ 3.9M)

Amperometric oxygen

Measurement parameters	– Dissolved oxygen: Saturation or concentration and temperature – Oxygen in gas: Concentration and temperature
Current range	Analog: 0 to –7000 nA
Oxygen measuring ranges, dissolved oxygen	– Saturation: 0 to 500 % air, 0 to 200 % O ₂ – Concentration: 0 ppb (µg/L) to 50.00 ppm (mg/L)
Oxygen measuring ranges, oxygen in gas	0 to 9999 ppm O ₂ gas, 0 to 100 vol % O ₂
Oxygen accuracy, dissolved oxygen ¹⁾	– Saturation: ±0.5 % of the measured value or ±0.5 %, depending on which is larger – Concentration at high values: ±0.5 % of the measured value or ±0.050 ppm/±0.050 mg/L, depending on which is larger – Concentration at low values: ±0.5 % of the measured value or ±0.001 ppm/±0.001 mg/L, depending on which is larger – Concentration at traces values: ±0.5 % of the measured value or ±0.100 ppb/±0.1 µg/L, depending on which is larger
Oxygen accuracy, oxygen in gas ¹⁾	– ±0.5 % of the measured value or ±5 ppb, depending on which is larger for ppm O ₂ gas – ±0.5 % of the measured value or ±0.01 %, depending on which is larger for vol % O ₂
Resolution current ¹⁾	Analog: 6 pA
Polarization voltage	– Analog: –1000 to 0 mV – ISM: –550 mV or – 674 mV (configurable)
Temperature input	NTC 22 kΩ, Pt1000, Pt100
Temperature compensation	Automatic
Temperature measuring range	– 10 to +80 °C (+ 14 to + 176 °F)
Temperature accuracy	±0.25 K in the range of – 10 to +80 °C (+ 14 to + 176 °F)
Max. sensor cable length	– Analog: 20 m (65 ft) – ISM: 80 m (260 ft)
Calibration	1-point (slope and offset) or process (slope and offset)

1) ISM input signal causes no additional error.

Optical oxygen

Measurement parameters	DO saturation or concentration and temperature
DO concentration range	0.1 ppb (µg/L) to 50.00 ppm (mg/L)
DO saturation range	0 to 500 % air, 0 to 100 % O ₂
DO resolution	Auto/0.001/0.01/0.1/1 (can be selected)
DO accuracy	±1 digit
Temperature measuring range	–30 to +150 °C (–22 to +302 °F)
Temperature resolution	Auto/0.001/0.01/0.1/1 (can be selected)
Temperature accuracy	±1 digit
Temperature repeatability	±1 digit
Temperature compensation	Automatic
Max. sensor cable length	15 m (50 ft)
Calibration	1-point (depending on sensor model), 2-point, process

Dissolved carbon dioxide

Measurement parameters	Dissolved carbon dioxide and temperature
CO ₂ measuring ranges	– 0 to 5000 mg/L – 0 to 200 %sat – 0 to 1500 mm Hg – 0 to 2000 mbar – 0 to 2000 hPa
CO ₂ accuracy	± 1 digit
CO ₂ resolution	Auto/0.001/0.01/0.1/1 (can be selected)
mV range	– 1500 to + 1500 mV
mV resolution	Auto/0.01/0.1/1 mV
mV accuracy	± 1 digit
Total pressure range (TotPres)	0 to 4000 mbar
Temperature input	Pt1000/NTC22K
Temperature measuring range	0 to + 60 °C (– 32 to + 140 °F)
Temperature resolution	Auto/0.001/0.01/0.1/1, (can be selected)
Temperature accuracy	± 1 digit
Temperature repeatability	± 1 digit
Max. sensor cable length	80 m (260 ft)
Calibration	1-point (offset), 2-point (slope or offset) or process (offset)

Available Buffer Sets

Buffer	MT-9 buffers with solution pH = 7.00 and pH = 9.21 @ 25 °C
--------	--

Thermal conductivity CO₂ (InPro 5500i)

CO ₂ measuring ranges	– 0 to 10 bar p (CO ₂)/0 to 145 psi p (CO ₂) – 0 to 15 g/L – 0 to 7 V/V CO ₂
Accuracy in fluids ¹⁾	– ± 1 % of reading (within ± 5 % of calibration temperature) – ± 2 % of reading over temperature range 0 to + 50 °C (+ 32 to + 122 °F)

Dissolved ozone

Measurement parameters	Concentration and temperature
Display range for current	0 to – 900 nA
Ozone measuring range	Concentration 0.1 ppb (µg/L) to 5.00 ppm (mg/L) O ₃
Ozone accuracy	± 1 digit
Resolution current	± 1 digit
Temperature compensation	Automatic
Temperature measuring range	0 to + 50 °C (– 32 to + 122 °F)
Temperature resolution	Auto/0.001/0.01/0.1/1 (can be selected)
Temperature accuracy	± 1 digit
Max. sensor cable length	80 m
Calibration	1-point ZeroPt or process (ZeroPt or slope)

16.2 Electrical Specifications

Display	Backlit LCD, 4 lines
Running capacity	Ca. 4 days
Keypad	5 tactile feedback keys
Languages	8 (English, German, French, Italian, Spanish, Portuguese, Russian and Japanese)
Connection terminals	Spring cage terminals, appropriate for wire cross section 0.2 to 1.5 mm ² (AWG 16 – 24)
Analog input	4 to 20 mA (for pressure compensation)

16.3 PROFIBUS PA Interface Specification

Supply voltage	<ul style="list-style-type: none"> – Non hazardous area (Non-IS): 9 to 32 V DC – Linear Barrier: 9 to 24 V DC – FISCO: 9 to 17.5 V DC
Current consumption	22 mA
Current consumption on error	< 28 mA
Number of current inputs	1 for pressure compensation
Profile	PROFIBUS PA 3.02
PA communication model	<ul style="list-style-type: none"> – 1 Resource Block – 1 Physical Block – 1 Analyser Transducer Block (Sensor Block) – 4 Analog Input Blocks – 1 Analog Output Block – 2 Discrete Input Blocks – 2 Discrete Output Blocks

16.4 Mechanical Specification

Dimensions	Housing –	144 × 144 × 116 mm
	Height × Width × Depth	(5.7 × 5.7 × 4.6 inch)
	Front bezel –	150 × 150 mm
	Height × Width	(5.9 × 5.9 inch)
	Max. depth – panel mounted	87 mm (excludes plug-in connectors)
Weight		1.50 kg (3.3 lb)
Material		Aluminum die cast
Enclosure rating		IP66/NEMA4X

16.5 Environmental Specifications

Storage temperature	–40 to +70 °C (–40 to +158 °F)
Ambient temperature operating range	–20 to +60 °C (–4 to +140 °F)
Relative humidity	0 to 95 % non-condensing
EMC	According to EN 61326-1 (general requirements) Emission: Class B, Immunity: Class A
Approvals and certificates	– ATEX/IECEx/UKCA Zone 1 Ex ib [ia Ga] IIC T4 Gb – cFMus Class I, Division 1, Groups A, B, C, D T4A – NEPSI EX Zone
CE mark	The measuring system is in conformity with the statutory requirements of the EC Directives. METTLER TOLEDO confirms successful testing of the device by affixing to it the CE mark.


16.6 Control Drawings


16.6.1 Installation, Maintenance and Inspection

1. Intrinsically Safe Apparatus can be a source of ignition if internal spacings are shorted or connections opened.
2. Although intrinsically safe circuits are inherently low energy, they may still present a shock hazard because of the operating voltage.
3. Refer to manufacturer's written instructions before working on associated apparatus.
4. Inspection should be performed periodically to ensure that intrinsic safety has not been compromised. Inspections should include reviewing for unauthorized modifications, corrosion, accidental damage, change of flammable materials, and the effects of aging.
5. User replaceable parts of an intrinsically safe system should not be replaced with other than the manufacturer's direct equivalent.
6. Maintenance work may be performed on energized apparatus in hazardous areas subject to the conditions as follows:
 - Disconnection of, and removal or replacement of, items of electrical apparatus and cabling if such action will not result in shorting of different intrinsically safe circuits.
 - Adjustment of any control that is necessary for the calibration of the electrical apparatus or system.
 - Only test instruments specified in the written instructions should be used.
 - Performance of other maintenance activities specifically permitted by the relevant control drawing and instruction manual.
7. Maintenance of Associated Apparatus and parts of intrinsically safe circuits located in unclassified areas should be restricted to that described in a way such that electrical apparatus or parts of circuits remain interconnected with parts of intrinsically safe systems located in hazardous areas. Safety barrier ground connections should not be removed without first disconnecting the hazardous-area circuits.
8. Other maintenance work on Associated Apparatus or parts of an intrinsically safe circuit mounted in an unclassified area should be performed only if the electrical apparatus or part of a circuit is disconnected from the part of the circuit located in a hazardous area.
9. The location classification and the suitability of the intrinsically safe system for that classification should be verified. This includes verifying that the class, group, and temperature ratings of both the Intrinsically Safe Apparatus and the Associated Apparatus agree with the actual classification of the location.

10. Prior to energizing, an intrinsically safe system should be inspected to ensure the following:
 - Installation is in compliance with the documentation;
 - Intrinsically safe circuits are properly separated from non-intrinsically safe circuits;
 - Cable shields are grounded in accordance with the installation documentation;
 - Modifications have been authorized;
 - Cables and wiring are not damaged;
 - Bonding and grounding connections are tight;
 - Bonding and grounding hardware is not corroded;
 - Resistance of any grounding conductor, including termination resistance from shunt-type-Associated Apparatus to the grounding electrode does not exceed one ohm;
 - Protection has not been defeated by bypassing; and
 - Check for signs of corrosion on the equipment and connections.
11. All deficiencies should be corrected.

16.6.2 Control Installation Drawing General Installation

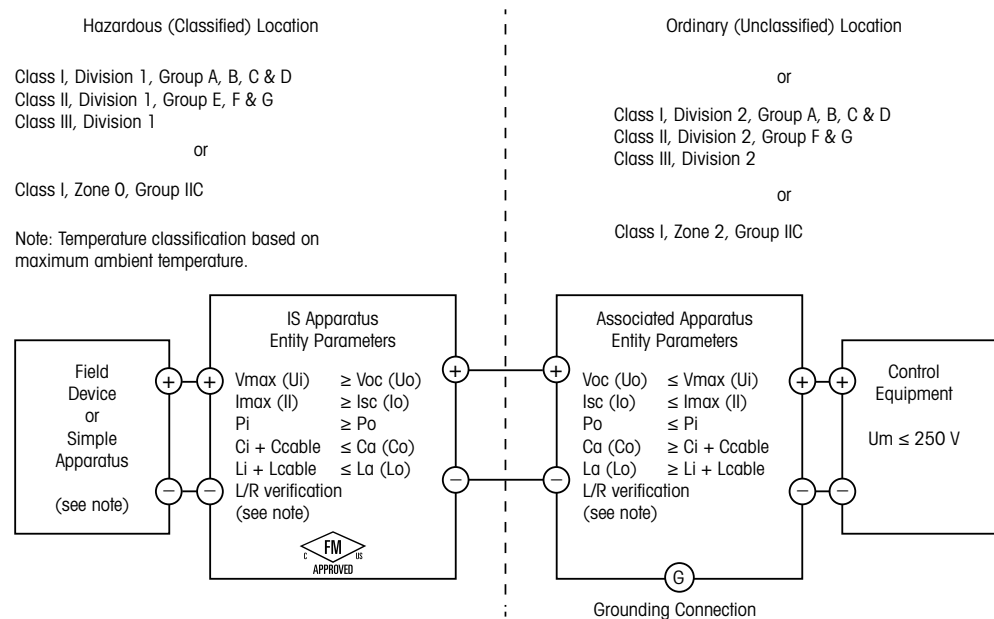

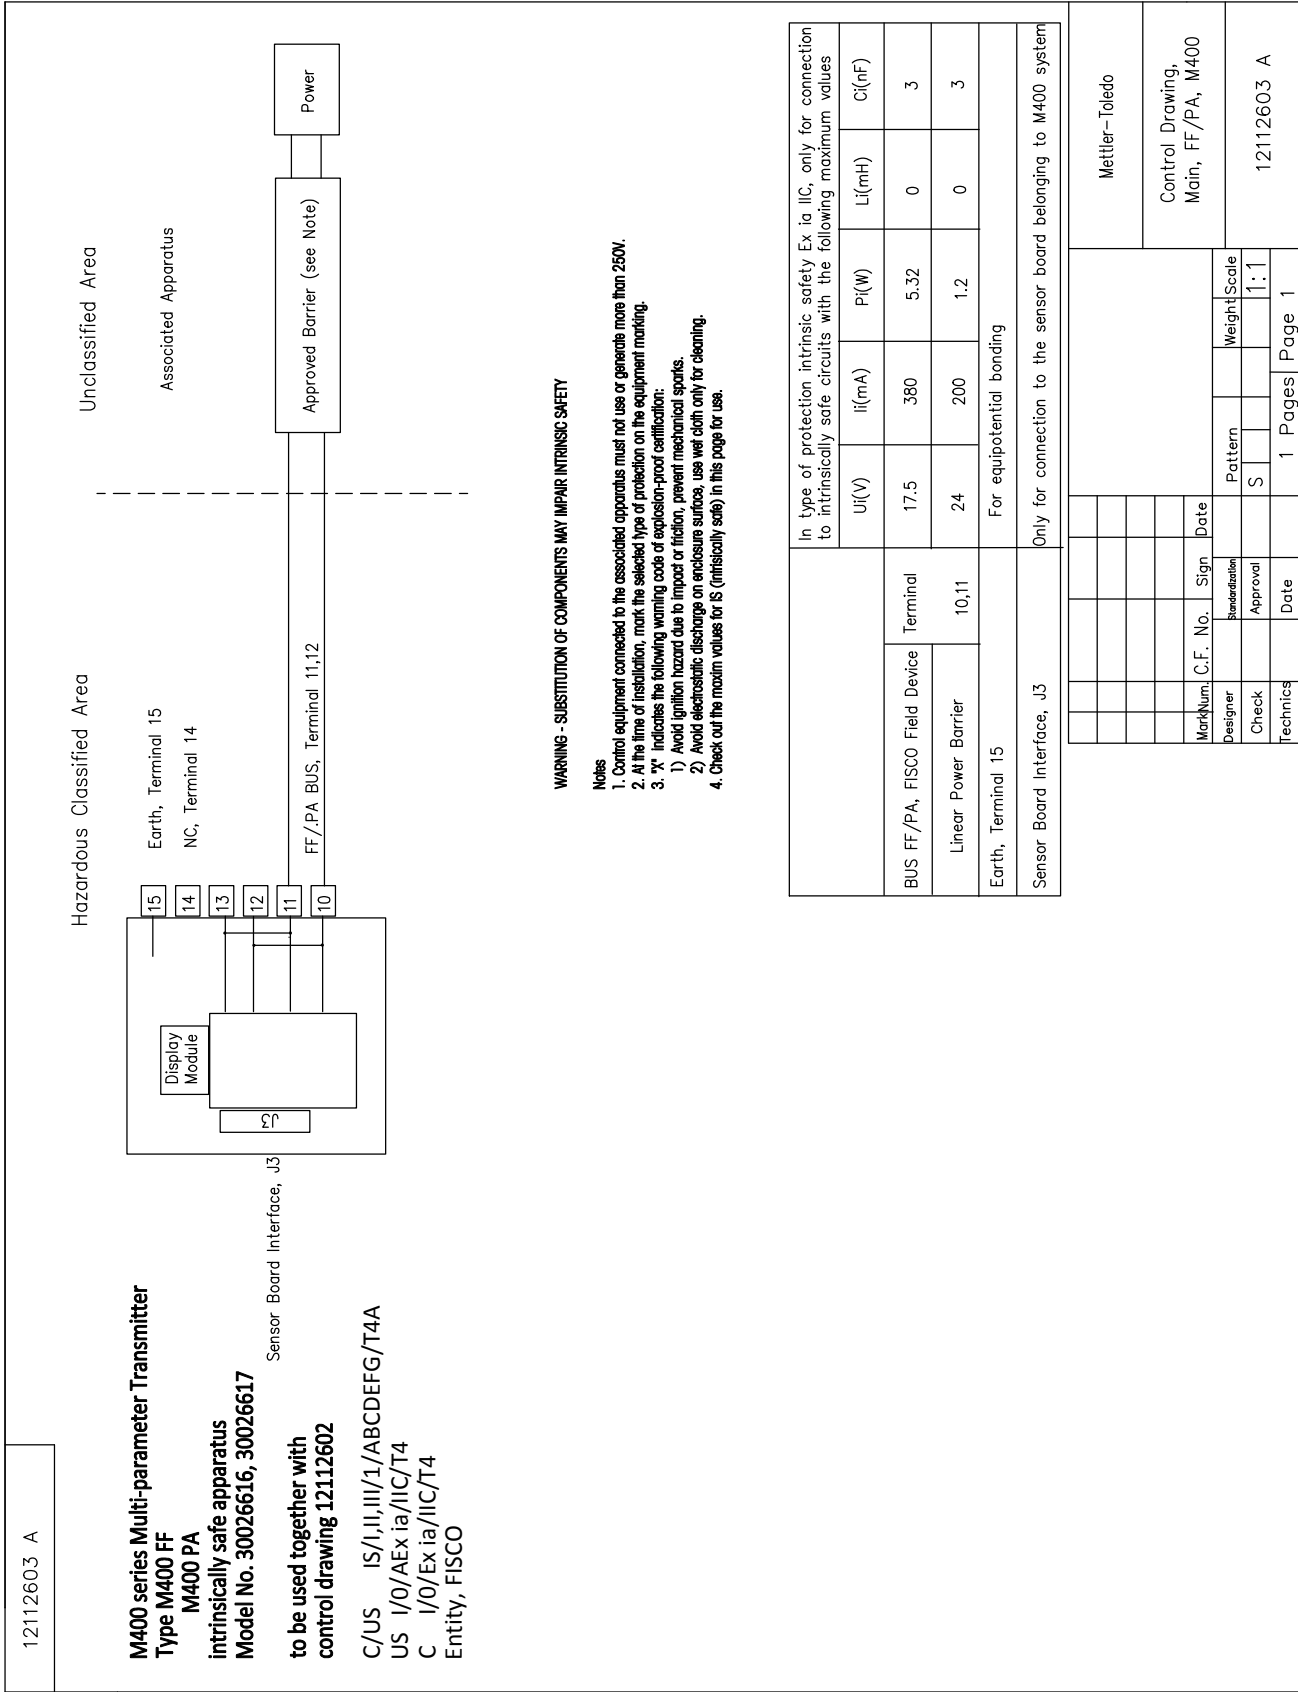


12112602 A

**Hazardous Classified Area
Sensor Board
belonging to
M400 Multi-parameter Transmitters
control drawing 12112601 or 12112603**

Sensor Interface	In type of protection intrinsic safety, only for connection to M400, with the following maximum values			
	U(V)	I(mA)	P(mW)	L(mH) C(uF)
pH measuring loop, Terminal A,E,G	Uo=5.88	Io=1.3	Po=1.9	Lo=5 Co=2.1
Conductivity measuring loop, Terminal A,B,E,G	Uo=5.88	Io=29	Po=4.3	Lo=1 Co=2.5
DO measuring loop, Terminal B,C,D,H	Uo=5.88	Io=29	Po=4.3	Lo=1 Co=2.5
Temperature measuring loop, Terminal I,J,K	Uo=5.88	Io=5.4	Po=8	Lo=5 Co=2
One-wire measuring loop, Terminal L,M	Uo=5.88	Io=22	Po=32	Lo=1 Co=2.8
485 measuring loop, Terminal N,O	Uo=5.88 Ui=30V	Io=54 Ii=100	Po=80 Pi=0.8	Lo=1 Li=0 Co=1.9 Ci=0.7
Analog input measuring loop, Terminal P,Q	Ui=30	Ii=100	Pi=800	Li=0 Ci=0.015

The measuring circuits are galvanically connected.

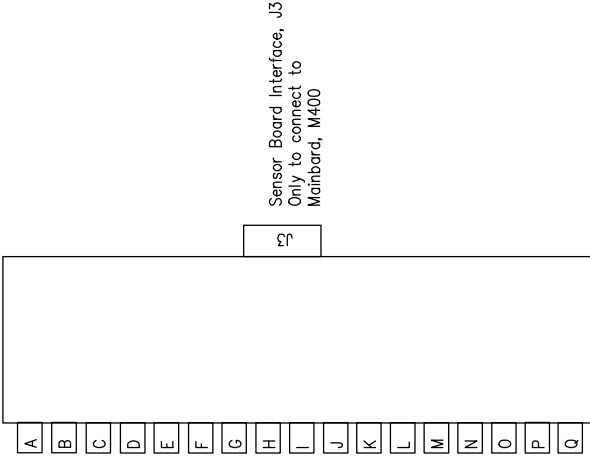

WARNING - SUBSTITUTION OF COMPONENTS MAY IMPAIR INTRINSIC SAFETY
WARNING - SUBSTITUTION OF COMPONENTS MAY IMPAIR THE SUITABILITY FOR ZONE 2

- Notes
IECEX, ATEX, FM, CSA
1. When installed in M400, intrinsically safe equipment connecting to A-Q must be approved or be a Simple Apparatus.
2. A Simple Apparatus is defined as a device that does not generate more than 1.5V, 0.1A or 25mW.
3. Check out the maximum values for IS (intrinsically safe) in this page for use.

MarkNum	C.F. No.	Sign	Date	Mettler-Toledo Instruments (Shanghai) Co. Ltd.		
Designer	Revision	Approval	Date	Control Drawing, Sensor, M400		
Check	Pattern	Weight	Scale	12112602 A		
Technics	S	1:1	1	1 Pages Page 1		

16.6.3 Notes

1. The intrinsic safety entity concept allows the interconnection of FM Approved intrinsically safe devices with entity parameters not specifically examined in combination as a system when: $V_{oc} (U_o) \text{ or } V_t \leq V_{max}$, $I_{sc} (I_o) \text{ or } I_t \leq I_{max}$, $C_a (C_o) \geq C_i + C_{cable}$, $L_a (L_o) \geq L_i + L_{cable}$, $P_o \leq P_i$
2. The intrinsic safety fieldbus intrinsically safe concept allows the interconnection of FM Approved intrinsically safe devices with fieldbus intrinsically safe concept parameters not specifically examined in combination as a system when: $V_{oc} (U_o) \text{ or } V_t < V_{max}$, $I_{sc} (I_o) \text{ or } I_t \leq I_{max}$, $P_o \leq P_i$
3. The configuration of associated apparatus must be FM Approved under the entity concept.
4. Associated Apparatus manufacturer's installation drawing must be followed when installing this equipment.
5. The configuration of field device sensor must be FM Approved under the entity concept.
6. The installation must be in accordance with the National Electrical Code. (ANSI/NFPA 70 (NEC.)), Articles 504 and 505, and ANSI/ISA-RP12.06.01, or the Canadian Electrical (CE) Code. (CEC Part 1, CAN/CSA-C22.1), Appendix F, and ANSI/ISARP12.06.01 when installed in Canada.
7. A dust-tight conduit seal must be used when installed in Class II and Class III environments.
8. Control equipment connected to the associated apparatus must not use or generate more than the maximum unclassified location voltage, U_m , or 250 VAC/DC.
9. Resistance between intrinsically safe ground and earth ground must be less than one ohm.
10. For Class I, Zone 0 and Division 1 locations, installation of the Multi-parameter Transmitter M400/2(X)H, M400G/2XH, M400FF, M400PA should be in accordance with ANSI/ISA RP12.06.01 "Installation of Intrinsically Safe Systems for Hazardous (Classified) Locations" and the National Electrical Code. (ANSI/ NRPA 70), or Canadian Electrical (CE) Code. (CEC Part 1, CAN/CSA-C22.1) when installed in Canada.
11. The Multi-parameter Transmitter M400/2(X)H, M400G/2XH, M400FF, M400PA are FM Approved for Class I, Zone 0 and Division 1 applications. If connecting [AEx ib] or [Ex ib] associated apparatus to the Multiparameter Transmitter M400/2(X)H, M400G/2XH, M400FF, M400PA, the above system is only suitable for Class I, Zone 1, and is not suitable for Class I, Zone 0, or Division 1 hazardous (classified) locations.
12. For Division 2 installations, the associated apparatus is not required to be FM Approved under entity concept if the Multi-parameter Transmitter M400/2(X)H, M400G/2XH is installed in accordance with the National Electrical Code. (ANSI/NFPA 70), Articles 504 and 505 or Canadian Electrical (CE) Code., CAN/CSA-C22.1, Part 1, Appendix F, for Division 2 wiring methods excluding nonincendive field wiring.
13. L_i may be greater than L_a and the cable length restrictions due to cable inductance (L_{cable}) can be ignored if both the following conditions are met: $L_a/R_a \text{ (or } L_o/R_o) > L_i/R_i$; $L_a/R_a \text{ (or } L_o/R_o) > L_{cable}/R_{cable}$
14. If the electrical parameters of the cable used are unknown, the following values may be used: Capacitance - 197 pF/m (60 pF/ft.); Inductance - 0.66 μ H/m (0.20 μ H/ft.)
15. Simple apparatus is defined as a device that does not generate more than 1.5 V, 0.1 A, or 25 mW.
16. No revision to the control installation drawing without prior authorization by FM Approvals.

17 Default Table

Common

Parameter	Sub parameter	Value	Unit
Measurement	Power failure	No	
	Software failure	No	
	ChB disconnected	Yes	
Clean	Interval time	0	hrs
	Clean time	0	sec
Language		English	
Passwords	Administrator	00000	
	Operator	00000	
Set/Clear LockOut		No	
Hold Output		Yes	
Display	Line1	a	
	Line2	b	
	Line3	c	
	Line4	d	
		On	
Name1	blank		
Name2	blank		
Resolution	Temperature	0.1	°C
	Conductivity	0.01	S/cm(Auto)
	Resistivity	0.01	Ω-cm(Auto)_
	pH	0.01	pH
	ORP	1.0	mV
	O ₂ ppb	1.	ppb
	O ₂ ppm	0.1	ppm
CIP Max		100	
CIP Temp		55 (30-100)	°C
SIP Max		100	
SIP Temp		115 (90-130)	°C
AutoClave Max		0	
ACT Initial		0	
TTM Initial		0	

pH

Parameter	Sub parameter	Value	Unit
Channel X	a	pH	pH
	b	Temperature	°C
	c	None	
	d	None	
Temperature source (for Analog sensor)		Auto	
pH buffer		Mettler-9	
Drift Control		Auto	
IP		7.0 (ISM sensor reading from sensor)	pH
STC		0.000	pH/°C
Fix CalTemp		No	
Cal constants (for Analog sensor)	pH	S = 100.0 %, Z = 7.000 pH	
	Temperature	M = 1.0, A = 0.0	
Cal constants (for ISM sensor)		Read from sensor	
Resolution	pH	0.01	pH
	Temperature	0.1	°C
Alarm	Rg diagnostics	Yes	
	Rr diagnostics	Yes	

pH/pNa

Parameter	Sub parameter	Value	Unit
Channel X	a	pH	pH
	b	Temperature	°C
	c	None	
	d	None	
Temperature source (for Analog sensor)		Auto	
pH buffer		Na+3.9M	
Drift Control		Auto	
IP		Reading form sensor	pH
STC		0.000	pH/°C
Fix CalTemp		No	
Cal constants		Read from sensor	
Resolution	pH	0.01	pH
	Temperature	0.1	°C
Alarm	Rg diagnostics	Yes	

Oxygen

Parameter	Sub parameter	Value	Unit
Channel X	a	O ₂	%air - O ₂ Hi ppb - O ₂ Lo, Trace ppm - Mec- Sens
	b	Temperature	°C
	c	None	
	d	None	°C
Temperature source (for Analog sensor)		UseNTC22K	
CalPres		759.8	mmHg
ProcPres		759.8	mmHg
ProcCalPres		CaPres	
Drift control		Auto	
Salinity		0.0	g/Kg
Humidity		100	%
Umeaspol		ISM: Read from sensor Analog: -674 for O ₂ Hi, others: -500.0	
Ucalpol		-674	mV
Cal constants (for Analog sensor)	O ₂ high	S = -70.00 nA, Z = 0.00 nA	
	O ₂ low	S = -350.00 nA, Z = 0.00 nA	
	O ₂ Trace	S = -4000.0 nA , Z = 0.00 nA	
	Temperature	M = 1.0, A = 0.0	
Cal constants (for ISM sensor)		Read from sensor	
Resolution	O ₂	0.1	%air
		1	ppb
	Temperature	0.1	°C
Alarm	Electrolyte low (ISM sensor)	Yes	

Resistivity/Conductivity

Parameter	Sub parameter	Value	Unit
Channel X	a	Conductivity	mS/cm
	b	Temperature	°C
	c	None	
	d	None	
Temperature source (for Analog sensor)		Auto	
Compensation		Standard	
Cal constants (for Analog sensor)	Cond/Res	M = 0.1, A = 0.0	
	Temperature	M = 1.0, A = 0.0	
Cal constants (for ISM sensor)		Read from sensor	
Resolution	Conductivity	0.01	mS/cm
	Temperature	0.1	°C
Alarm	Cond cell shorted	No	
	Dry cond sensor	No	
	Cell deviation (ISM sensor)	No	

CO₂

Parameter	Sub parameter	Value	Unit
Channel X	a	%CO ₂	%CO ₂
	b	Temperature	°C
	c	----	
	d	----	
Temperature source (for Analog sensor)		Auto	
pH buffer		Mettler-9	
Drift Control		Auto	
Salinity		28.0	g/L
HCO ₃		0.05	mol/L
TotPres		750.1	mmHg
Cal constants	CO ₂	Read from sensor	
Resolution	CO ₂	0.1	hPa
	Temperature	0.1	°C
Alarm	Rg diagnostics	No	

Ozone

Parameter	Sub parameter	Value	Unit
Channel X	a	O ₃	ppb
	b	Temperature	°C
	c	----	
	d	----	
SAN Max Cycles		Read from sensor	
Conc. Max		Read from sensor	
Conc. Min		Read from sensor	
Cycle Time		Read from sensor	
Resolution	O ₃	1	ppb
	Temperature	0.1	°C
Alarm	Rg diagnostics	No	

18 Warranty

METTLER TOLEDO warrants this product to be free from significant deviations in material and workmanship for a period of one year from the date of purchase. If repair is necessary and not the result of abuse or misuse within the warranty period, please return by freight pre-paid and amendment will be made without any charge. METTLER TOLEDO's Customer Service Dept. will determine if the product problem is due to deviations or customer abuse. Out-of-warranty products will be repaired on an exchange basis at cost.

The above warranty is the only warranty made by METTLER TOLEDO and is lieu of all other warranties, expressed or implied, including, without limitation, implied warranties of merchantability and fitness for a particular purpose. METTLER TOLEDO shall not be liable for any loss, claim, expense or damage caused by, contributed to or arising out of the acts or omissions of the Buyer or Third Parties, whether negligent or otherwise. In no event shall METTLER TOLEDO's liability for any cause of action whatsoever exceed the cost of the item giving rise to the claim, whether based in contract, warranty, indemnity, or tort (including negligence).

19 Buffer Tables

M400 transmitters have the ability to do automatic pH buffer recognition. The following tables show different standard buffers that are automatically recognized.

19.1 Standard pH Buffers

19.1.1 Mettler-9

Temp (°C)	pH of buffer solutions			
0	2.03	4.01	7.12	9.52
5	2.02	4.01	7.09	9.45
10	2.01	4.00	7.06	9.38
15	2.00	4.00	7.04	9.32
20	2.00	4.00	7.02	9.26
25	2.00	4.01	7.00	9.21
30	1.99	4.01	6.99	9.16
35	1.99	4.02	6.98	9.11
40	1.98	4.03	6.97	9.06
45	1.98	4.04	6.97	9.03
50	1.98	4.06	6.97	8.99
55	1.98	4.08	6.98	8.96
60	1.98	4.10	6.98	8.93
65	1.98	4.13	6.99	8.90
70	1.99	4.16	7.00	8.88
75	1.99	4.19	7.02	8.85
80	2.00	4.22	7.04	8.83
85	2.00	4.26	7.06	8.81
90	2.00	4.30	7.09	8.79
95	2.00	4.35	7.12	8.77

19.1.2 Mettler-10

Temp (°C)	pH of buffer solutions				
0	2.03	4.01	7.12	10.65	
5	2.02	4.01	7.09	10.52	
10	2.01	4.00	7.06	10.39	
15	2.00	4.00	7.04	10.26	
20	2.00	4.00	7.02	10.13	
25	2.00	4.01	7.00	10.00	
30	1.99	4.01	6.99	9.87	
35	1.99	4.02	6.98	9.74	
40	1.98	4.03	6.97	9.61	
45	1.98	4.04	6.97	9.48	
50	1.98	4.06	6.97	9.35	
55	1.98	4.08	6.98		
60	1.98	4.10	6.98		
65	1.98	4.13	6.99		
70	1.99	4.16	7.00		
75	1.99	4.19	7.02		
80	2.00	4.22	7.04		
85	2.00	4.26	7.06		
90	2.00	4.30	7.09		
95	2.00	4.35	7.12		

19.1.3 NIST Technical Buffers

Temp (°C)	pH of buffer solutions				
0	1.67	4.00	7.115	10.32	13.42
5	1.67	4.00	7.085	10.25	13.21
10	1.67	4.00	7.06	10.18	13.01
15	1.67	4.00	7.04	10.12	12.80
20	1.675	4.00	7.015	10.07	12.64
25	1.68	4.005	7.00	10.01	12.46
30	1.68	4.015	6.985	9.97	12.30
35	1.69	4.025	6.98	9.93	12.13
40	1.69	4.03	6.975	9.89	11.99
45	1.70	4.045	6.975	9.86	11.84
50	1.705	4.06	6.97	9.83	11.71
55	1.715	4.075	6.97		11.57
60	1.72	4.085	6.97		11.45
65	1.73	4.10	6.98		
70	1.74	4.13	6.99		
75	1.75	4.14	7.01		
80	1.765	4.16	7.03		
85	1.78	4.18	7.05		
90	1.79	4.21	7.08		
95	1.805	4.23	7.11		

19.1.4 NIST Standard Buffers (DIN and JIS 19266: 2000–01)

Temp (°C)	pH of buffer solutions			
0				
5	1.668	4.004	6.950	9.392
10	1.670	4.001	6.922	9.331
15	1.672	4.001	6.900	9.277
20	1.676	4.003	6.880	9.228
25	1.680	4.008	6.865	9.184
30	1.685	4.015	6.853	9.144
37	1.694	4.028	6.841	9.095
40	1.697	4.036	6.837	9.076
45	1.704	4.049	6.834	9.046
50	1.712	4.064	6.833	9.018
55	1.715	4.075	6.834	8.985
60	1.723	4.091	6.836	8.962
70	1.743	4.126	6.845	8.921
80	1.766	4.164	6.859	8.885
90	1.792	4.205	6.877	8.850
95	1.806	4.227	6.886	8.833



NOTE: The pH(S) values of the individual charges of the secondary reference materials are documented in a certificate of an accredited laboratory. This certificate is supplied with the respective buffer materials. Only these pH(S) values shall be used as standard values for the secondary reference buffer materials. Correspondingly, this standard does not include a table with standard pH values for practical use. The table above only provides examples of pH(PS) values for orientation.

19.1.5 Hach Buffers

Buffer values up to 60 °C as specified by Bergmann & Beving Process AB.

Temp (°C)	pH of buffer solutions		
0	4.00	7.14	10.30
5	4.00	7.10	10.23
10	4.00	7.04	10.11
15	4.00	7.04	10.11
20	4.00	7.02	10.05
25	4.01	7.00	10.00
30	4.01	6.99	9.96
35	4.02	6.98	9.92
40	4.03	6.98	9.88
45	4.05	6.98	9.85
50	4.06	6.98	9.82
55	4.07	6.98	9.79
60	4.09	6.99	9.76

19.1.6 Ciba (94) Buffers

Temp (°C)	pH of buffer solutions				
0	2.04	4.00	7.10	10.30	
5	2.09	4.02	7.08	10.21	
10	2.07	4.00	7.05	10.14	
15	2.08	4.00	7.02	10.06	
20	2.09	4.01	6.98	9.99	
25	2.08	4.02	6.98	9.95	
30	2.06	4.00	6.96	9.89	
35	2.06	4.01	6.95	9.85	
40	2.07	4.02	6.94	9.81	
45	2.06	4.03	6.93	9.77	
50	2.06	4.04	6.93	9.73	
55	2.05	4.05	6.91	9.68	
60	2.08	4.10	6.93	9.66	
65	2.07*	4.10*	6.92*	9.61*	
70	2.07	4.11	6.92	9.57	
75	2.04*	4.13*	6.92*	9.54*	
80	2.02	4.15	6.93	9.52	
85	2.03*	4.17*	6.95*	9.47*	
90	2.04	4.20	6.97	9.43	
95	2.05*	4.22*	6.99*	9.38*	

* Extrapolated

19.1.7 Merck Titrisole, Riedel-de-Haën Fixanale

Temp (°C)	pH of buffer solutions				
0	2.01	4.05	7.13	9.24	12.58
5	2.01	4.05	7.07	9.16	12.41
10	2.01	4.02	7.05	9.11	12.26
15	2.00	4.01	7.02	9.05	12.10
20	2.00	4.00	7.00	9.00	12.00
25	2.00	4.01	6.98	8.95	11.88
30	2.00	4.01	6.98	8.91	11.72
35	2.00	4.01	6.96	8.88	11.67
40	2.00	4.01	6.95	8.85	11.54
45	2.00	4.01	6.95	8.82	11.44
50	2.00	4.00	6.95	8.79	11.33
55	2.00	4.00	6.95	8.76	11.19
60	2.00	4.00	6.96	8.73	11.04
65	2.00	4.00	6.96	8.72	10.97
70	2.01	4.00	6.96	8.70	10.90
75	2.01	4.00	6.96	8.68	10.80
80	2.01	4.00	6.97	8.66	10.70
85	2.01	4.00	6.98	8.65	10.59
90	2.01	4.00	7.00	8.64	10.48
95	2.01	4.00	7.02	8.64	10.37

19.1.8 WTW Buffers

Temp (°C)	pH of buffer solutions			
0	2.03	4.01	7.12	10.65
5	2.02	4.01	7.09	10.52
10	2.01	4.00	7.06	10.39
15	2.00	4.00	7.04	10.26
20	2.00	4.00	7.02	10.13
25	2.00	4.01	7.00	10.00
30	1.99	4.01	6.99	9.87
35	1.99	4.02	6.98	9.74
40	1.98	4.03	6.97	9.61
45	1.98	4.04	6.97	9.48
50	1.98	4.06	6.97	9.35
55	1.98	4.08	6.98	
60	1.98	4.10	6.98	
65	1.99	4.13	6.99	
70		4.16	7.00	
75		4.19	7.02	
80		4.22	7.04	
85		4.26	7.06	
90		4.30	7.09	
95		4.35	7.12	

19.1.9 JIS Z 8802 Buffers

Temp (°C)	pH of buffer solutions			
0	1.666	4.003	6.984	9.464
5	1.668	3.999	6.951	9.395
10	1.670	3.998	6.923	9.332
15	1.672	3.999	6.900	9.276
20	1.675	4.002	6.881	9.225
25	1.679	4.008	6.865	9.180
30	1.683	4.015	6.853	9.139
35	1.688	4.024	6.844	9.102
38	1.691	4.030	6.840	9.081
40	1.694	4.035	6.838	9.068
45	1.700	4.047	6.834	9.038
50	1.707	4.060	6.833	9.011
55	1.715	4.075	6.834	8.985
60	1.723	4.091	6.836	8.962
70	1.743	4.126	6.845	8.921
80	1.766	4.164	6.859	8.885
90	1.792	4.205	6.877	8.850
95	1.806	4.227	6.886	8.833

19.2 Dual Membrane pH Electrode Buffers

19.2.1 Mettler-pH/pNa Buffers (Na+ 3.9M)

Temp (°C)	pH of buffer solutions			
0	1.98	3.99	7.01	9.51
5	1.98	3.99	7.00	9.43
10	1.99	3.99	7.00	9.36
15	1.99	3.99	6.99	9.30
20	1.99	4.00	7.00	9.25
25	2.00	4.01	7.00	9.21
30	2.00	4.02	7.01	9.18
35	2.01	4.04	7.01	9.15
40	2.01	4.05	7.02	9.12
45	2.02	4.07	7.03	9.11
50	2.02	4.09	7.04	9.10

For addresses of METTLER TOLEDO
Market Organizations please go to:
www.mt.com/contacts

www.mt.com/pro

For more information



Management System
certified according to
ISO 9001/ISO 14001



METTLER TOLEDO Group
Process Analytics
Local contact: www.mt.com/contacts

Subject to technical changes
© 02/2023 METTLER TOLEDO
All rights reserved
Printed in Switzerland. 30 134 634 F

